

Sample Name : [Arg8]-Vasopressin (AVP)  
 Cat No. : RP20275  
 Lot No. : E1701119J  
 Time Processed : 17:39:02  
 Month-Day-Year Processed : 10/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK12010012

<Chromatogram>

mV

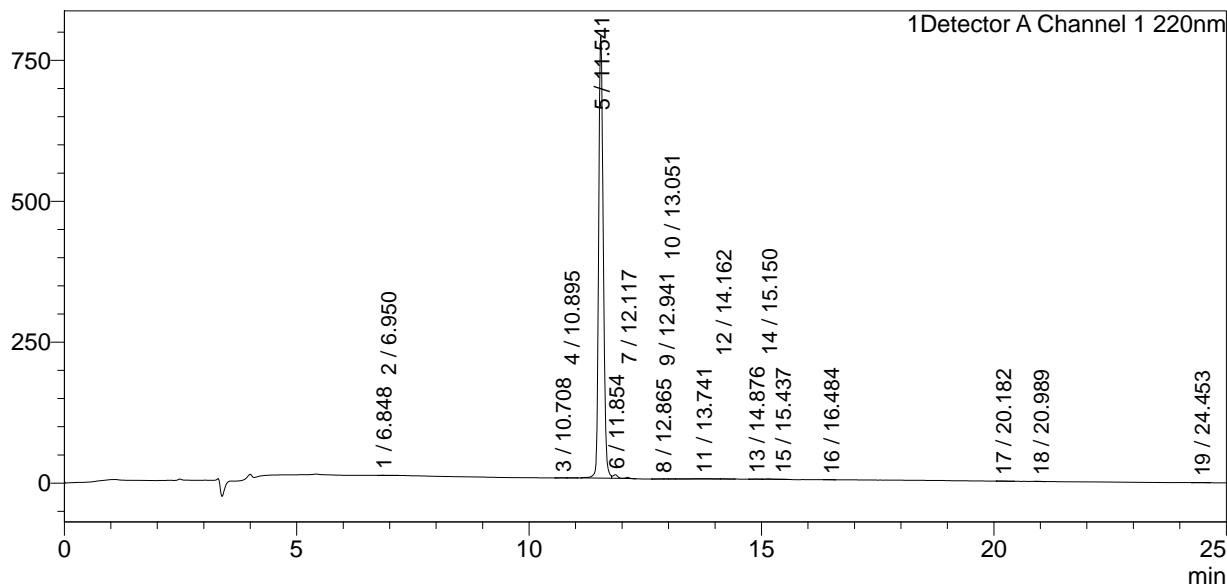

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.848	2639	392	0.048
2	6.950	4592	300	0.083
3	10.708	1862	206	0.034
4	10.895	1541	162	0.028
5	11.541	5422365	783369	97.737
6	11.854	43438	6240	0.783
7	12.117	10742	1942	0.194
8	12.865	3196	319	0.058
9	12.941	1830	333	0.033
10	13.051	2628	312	0.047
11	13.741	29611	753	0.534
12	14.162	3599	399	0.065
13	14.876	2454	274	0.044
14	15.150	5477	716	0.099
15	15.437	1242	155	0.022

Peak#	Ret. Time	Area	Height	Area%
16	16.484	1335	184	0.024
17	20.182	1357	116	0.024
18	20.989	2221	410	0.040
19	24.453	5810	658	0.105
Total		5547938	797240	100.000