

Sample Name :Oxytocin
 Cat No.: RP10407
 Lot No.: E4927520G
 Time Processed :14:51:33
 Month-Day-Year Processed :07/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

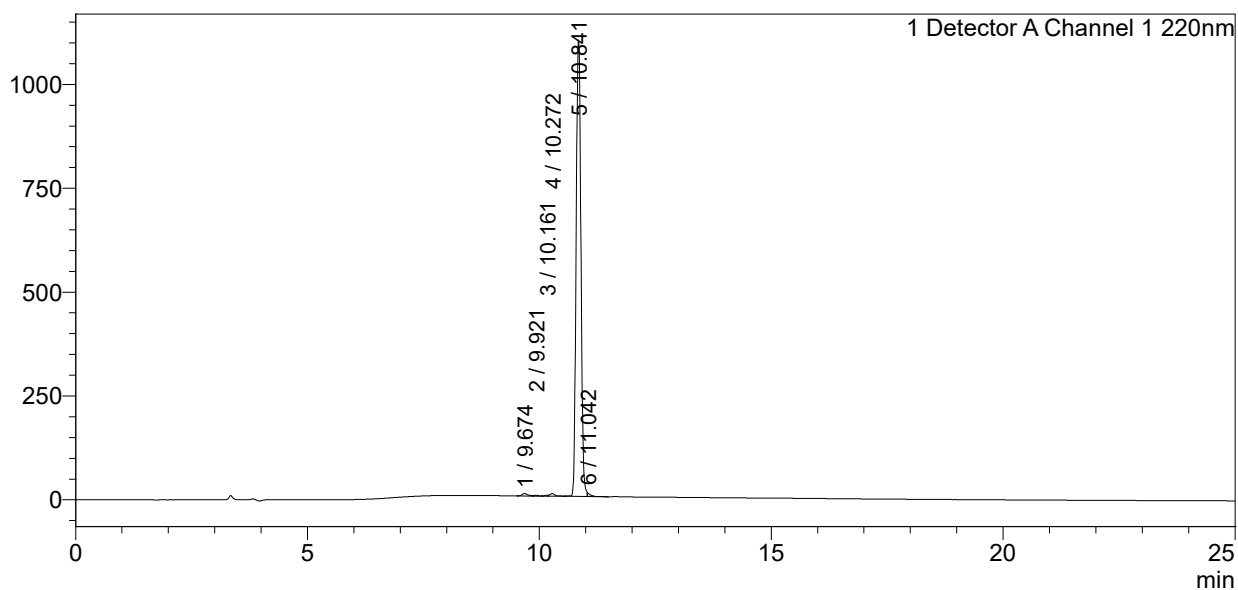

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.674	49788	5673	0.620
2	9.921	13551	1893	0.169
3	10.161	12767	2485	0.159
4	10.272	50521	6576	0.629
5	10.841	7861757	1099122	97.920
6	11.042	40401	9067	0.503
Total		8028785	1124817	100.000