

Sample Name :Neurotensin
 Cat No. :RP10439
 Lot No. :E9660419L
 Time Processed :4:10:57
 Month-Day-Year Processed :12/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

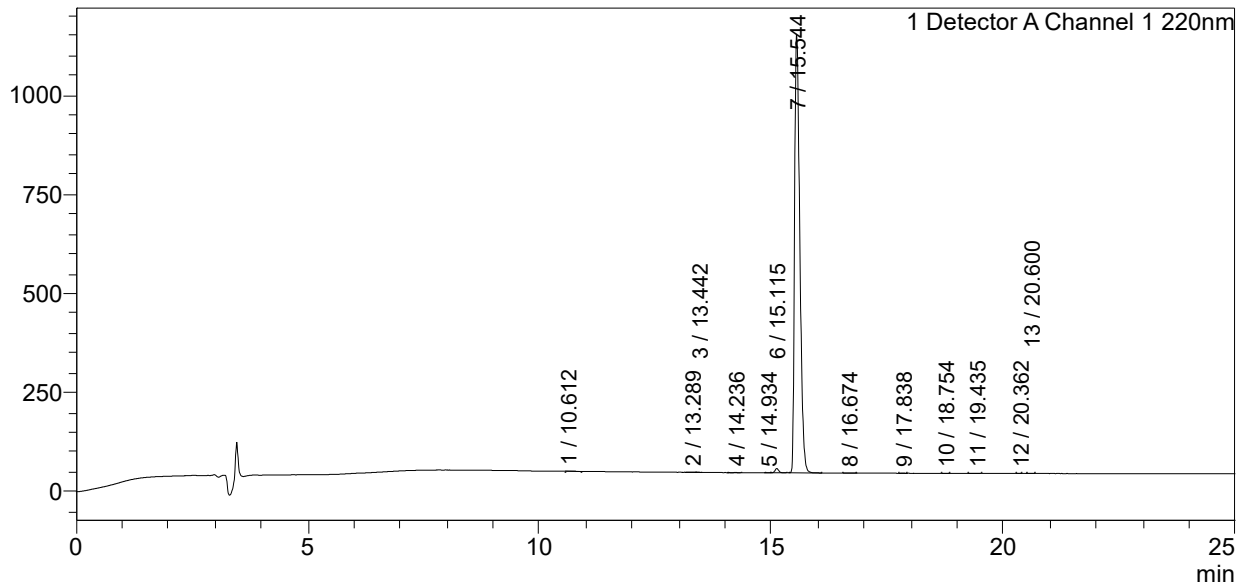

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.612	3984	558	0.045
2	13.289	2499	356	0.028
3	13.442	1283	194	0.015
4	14.236	3295	437	0.038
5	14.934	2064	520	0.024
6	15.115	62114	11056	0.707
7	15.544	8696698	1106316	99.028
8	16.674	2185	264	0.025
9	17.838	1668	311	0.019
10	18.754	1090	253	0.012
11	19.435	2044	243	0.023
12	20.362	1185	271	0.013
13	20.600	1942	331	0.022
Total		8782051	1121112	100.000