

Sample Name :Bactenecin, bovine
 Cat. No. :RP11235
 Lot. No. :E3658020J
 Time Processed : 7:47:29 AM
 Month-Day-Year Processed : 11/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


| Time | Module | Command | Value |
|-------|------------|---------|-------|
| 0.01 | Pumps | B.Conc | 5 |
| 25.00 | Pumps | B.Conc | 65 |
| 25.01 | Pumps | B.Conc | 95 |
| 32.00 | Pumps | B.Conc | 95 |
| 32.01 | Pumps | B.Conc | 5 |
| 40.00 | Pumps | B.Conc | 5 |
| 45.00 | Controller | Stop | |

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

mV

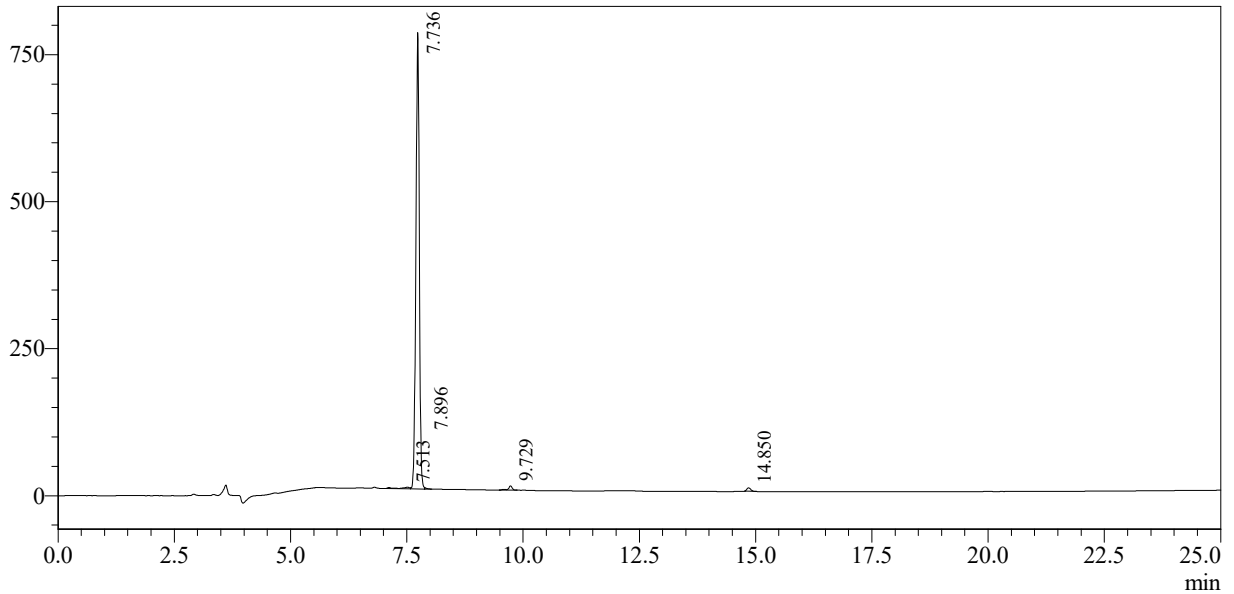

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 7.513 | 38000 | 2852 | 0.924 |
| 2 | 7.736 | 3988438 | 775885 | 97.003 |
| 3 | 7.896 | 6425 | 2085 | 0.156 |
| 4 | 9.729 | 43850 | 7326 | 1.066 |
| 5 | 14.850 | 34965 | 5957 | 0.850 |
| Total | | 4111678 | 794105 | 100.000 |