


Mass Spectrum

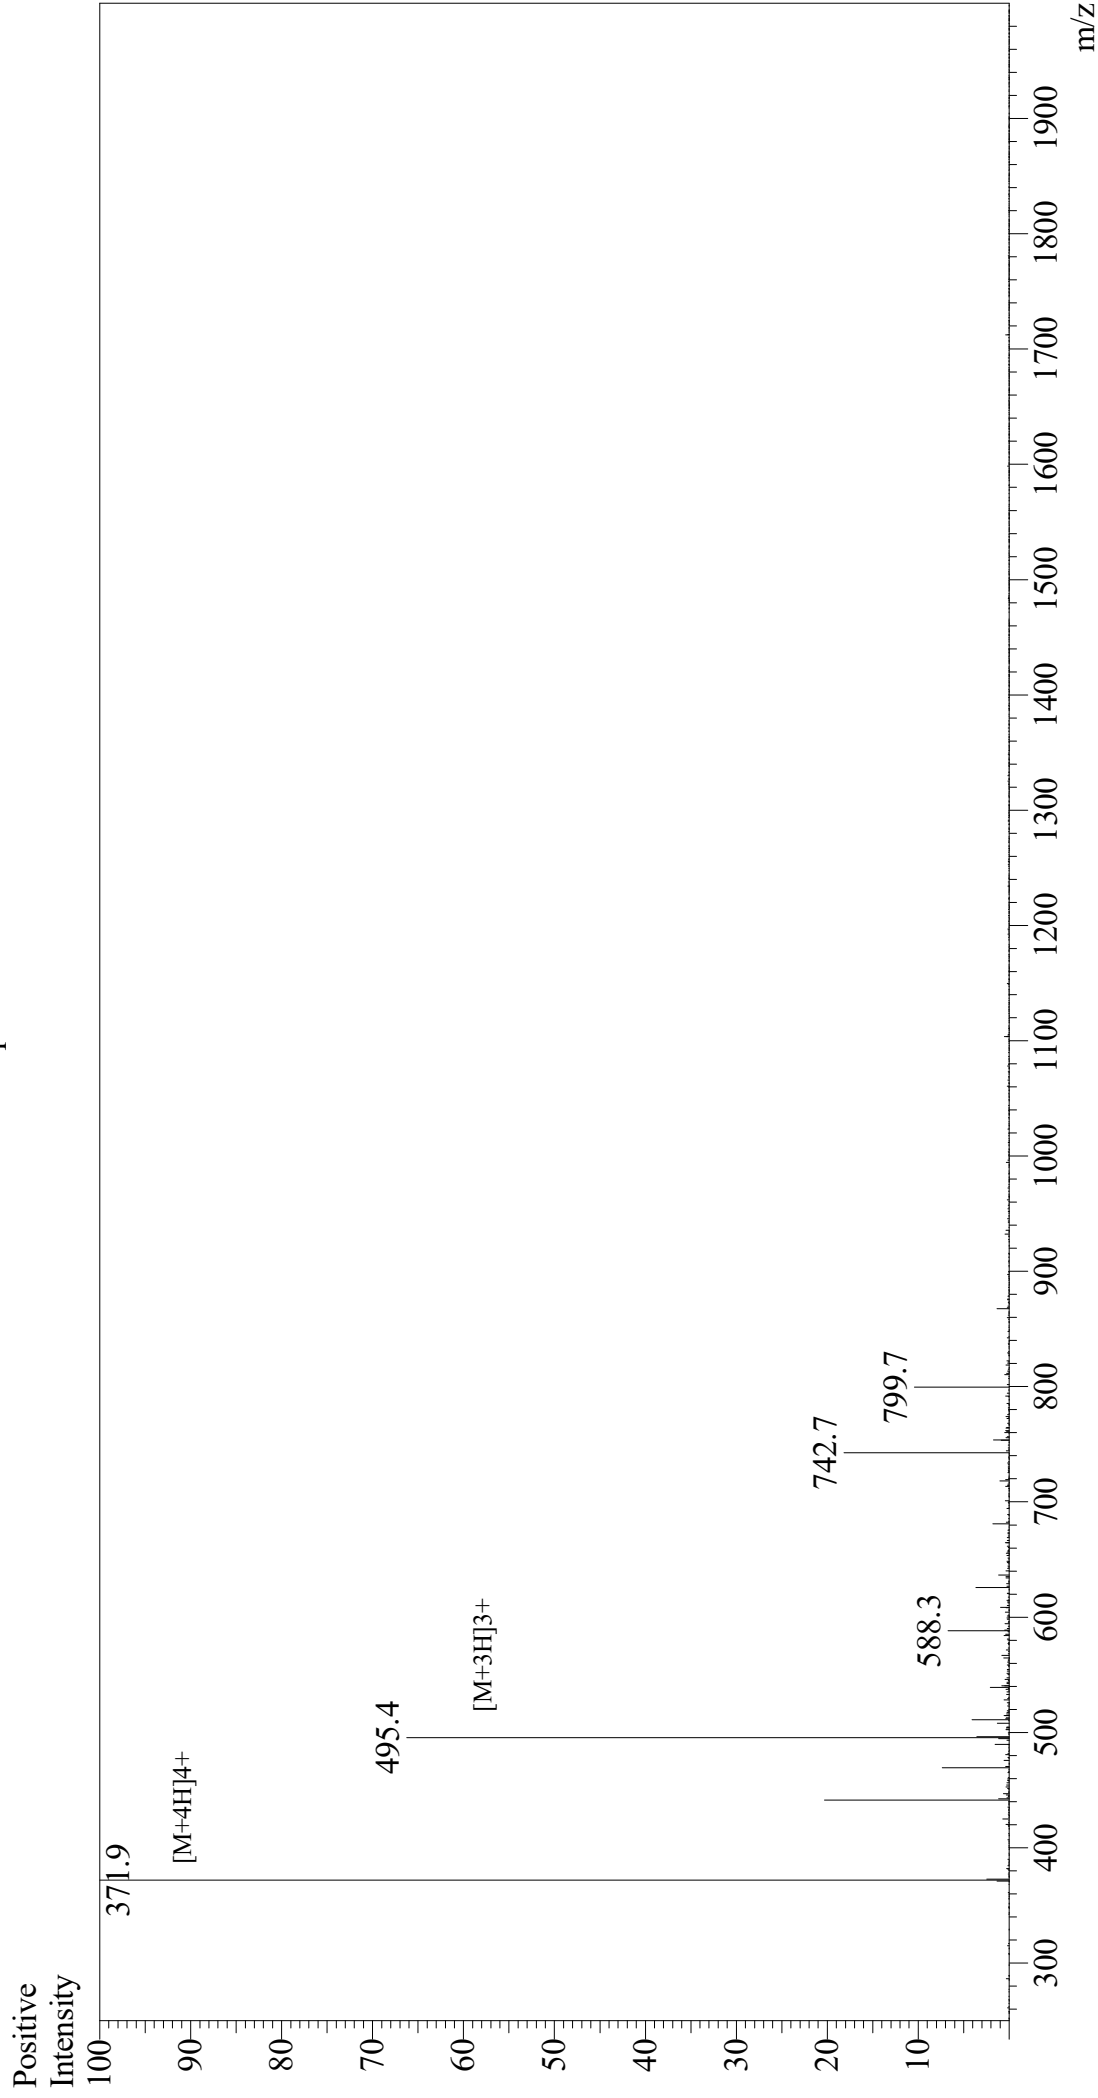

Sample Information

Month-Day Processed : 11/20/20
Time Processed : 08:37:02 PM
Injection Volume : 0.3
Sample Name : Bactenecin, bovine
Cat No. : RP11235
Lot No. : E3658020J
Theoretical MW : 1483.90
Observed MW : 1483.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH