

Sample Name :HA Peptide
 Cat. No.: RP11735
 Lot. No. : E0909419G
 Time Processed :7:44:53
 Month-Day-Year Processed :07/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

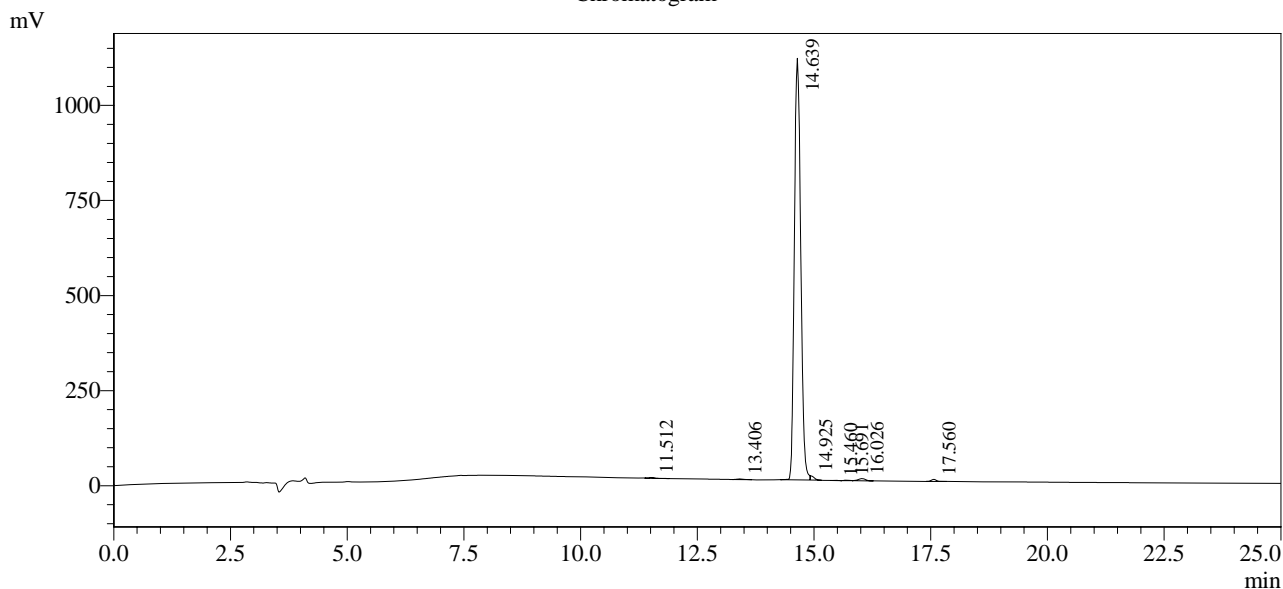

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.512	16965	2123	0.157
2	13.406	14886	1604	0.138
3	14.639	10576670	1108753	98.091
4	14.925	62121	11250	0.576
5	15.460	3529	646	0.033
6	15.691	8722	1340	0.081
7	16.026	59451	5691	0.551
8	17.560	40120	5351	0.372
Total		10782465	1136758	100.000