


Mass Spectrum

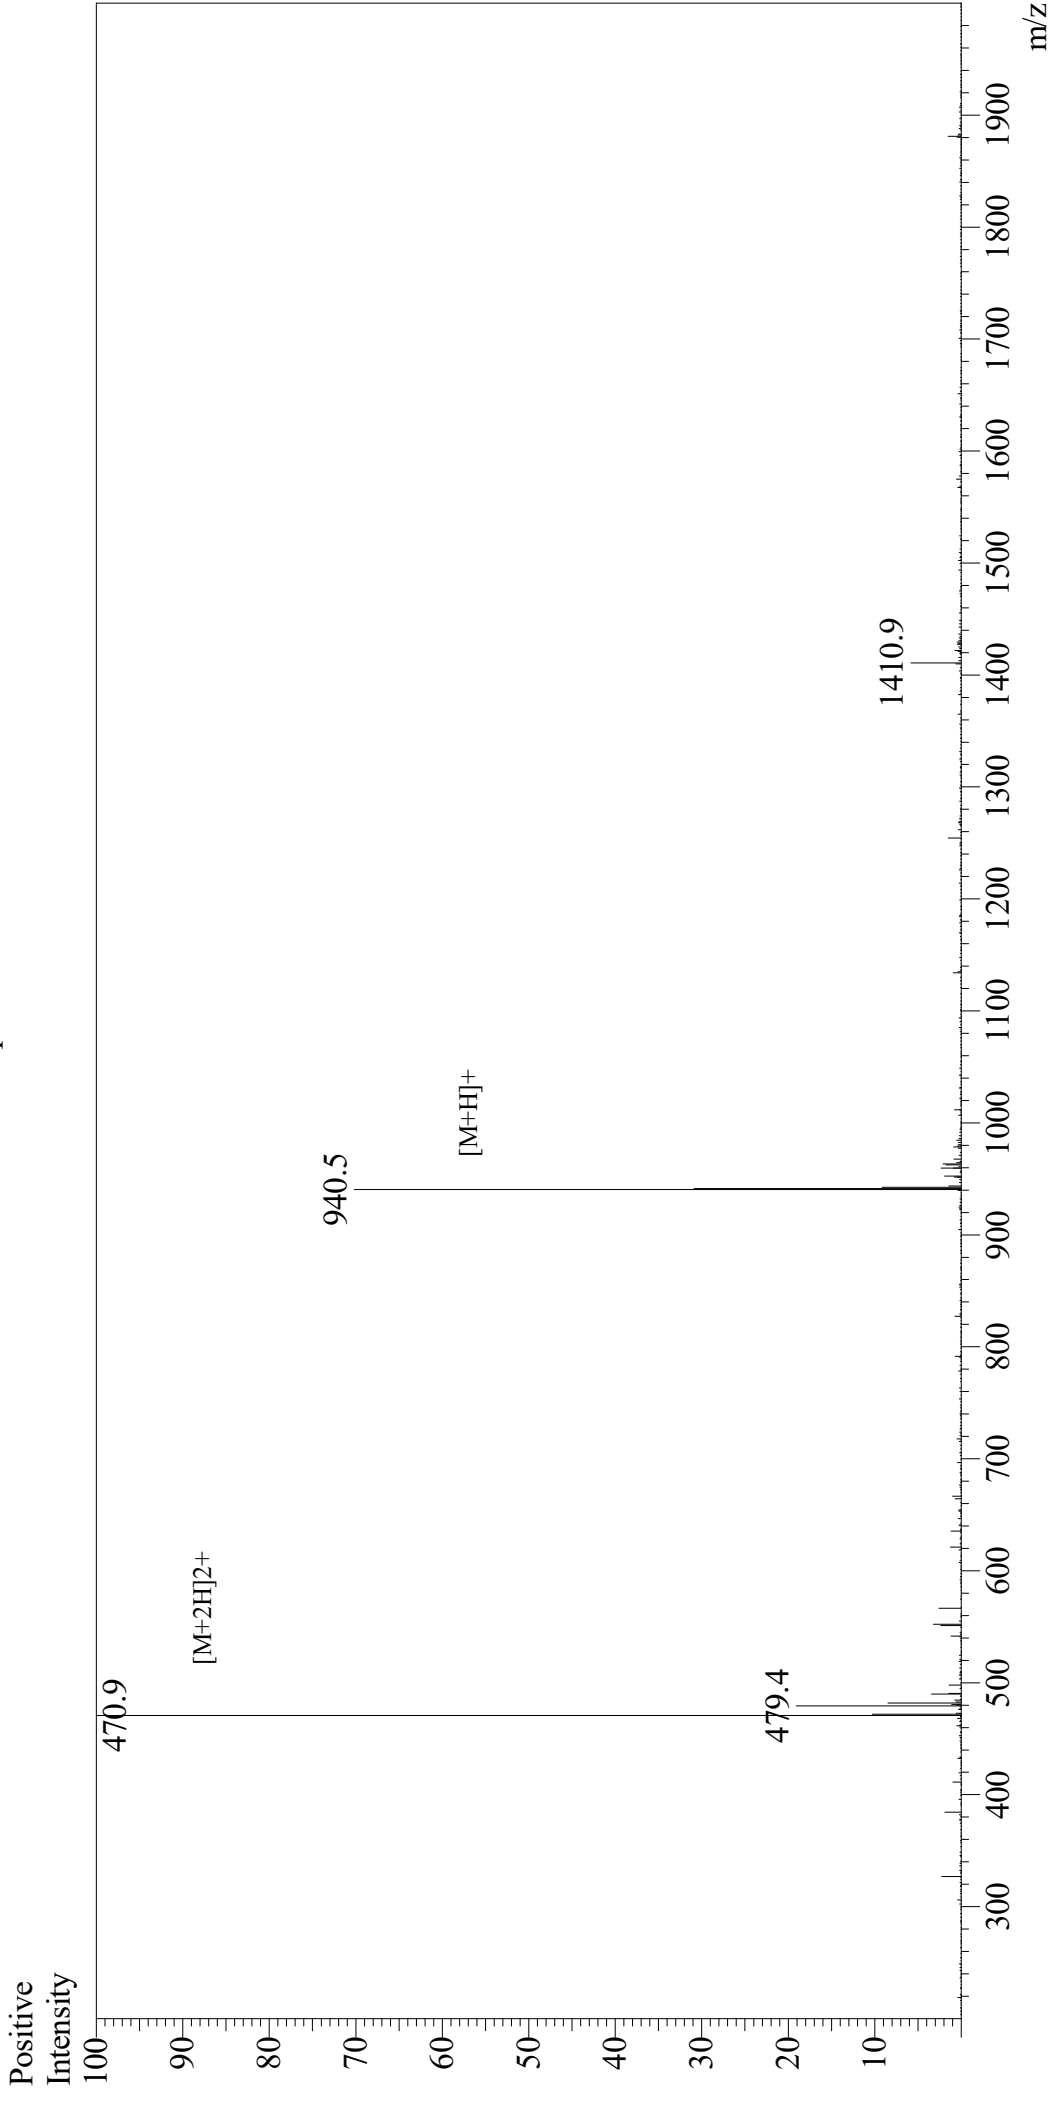

Sample Information

User :	Gary	Equipment	: GK11010007
Month-Day Processed :	03/28/20	Interface Bias	: +4.5kV
Time Processed :	09:19:56 AM	Drying Gas Flow	: 5 L/min
Injection Volume :	0.3	T.Flow	: 0.2ml/min
Sample Name :	Influenza HA (518-526)	B.conc	: 50%H ₂ O/50%MeOH
Cat No. :	RP20284		
Lot No. :	E3617020C		
Theoretical MW :	940.05		
Observed MW :	939.8		