

Sample Name : Kassinin
 Cat. No. : RP10461
 Lot. No. : E4805919I
 Time Processed : 13:01:00
 Month-Day-Year Processed : 09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

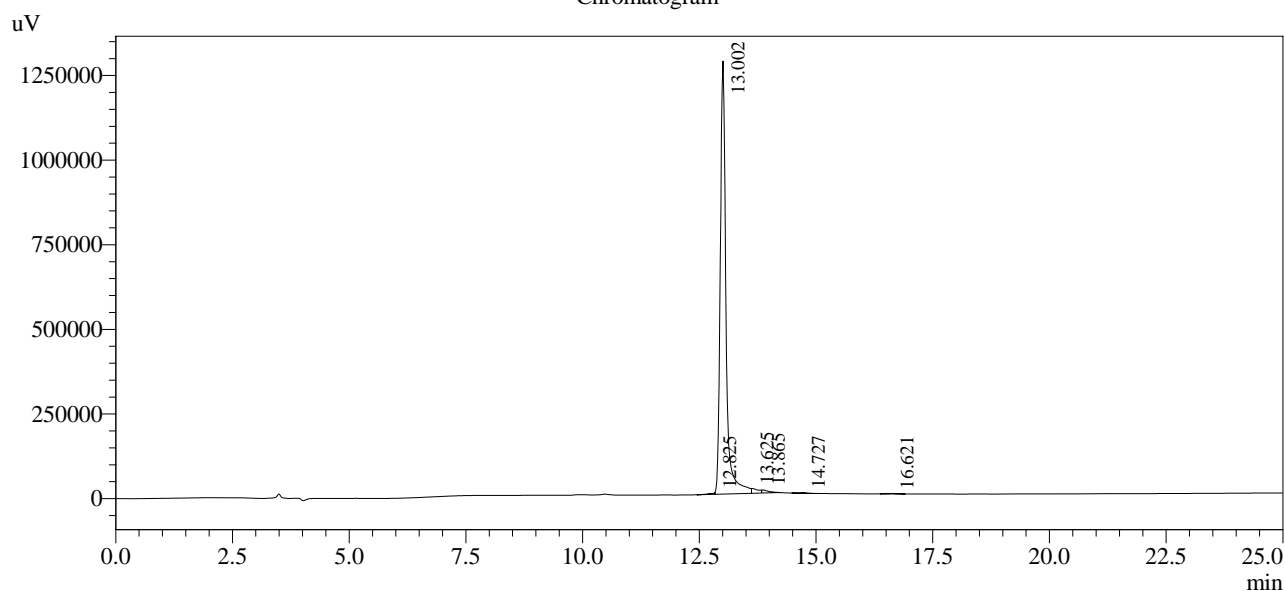

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.825	34137	4006	0.305
2	13.002	10902843	1279533	97.429
3	13.625	138949	14179	1.242
4	13.865	92465	9132	0.826
5	14.727	8874	1418	0.079
6	16.621	13229	1337	0.118
Total		11190498	1309604	100.000