

Sample Name : hgp100(25-33)
 Cat. No. : RP20344
 Lot. No. : PE4071612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

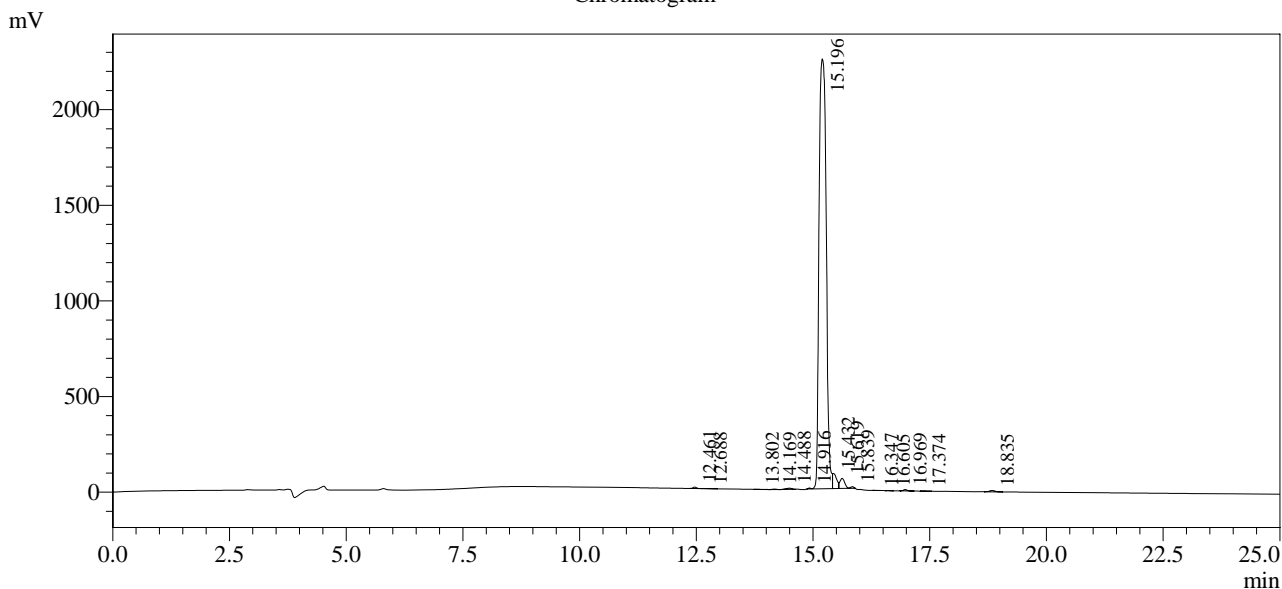

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.461	38133	7315	0.152
2	12.688	4819	534	0.019
3	13.802	4073	478	0.016
4	14.169	13544	2331	0.054
5	14.488	59119	6294	0.236
6	14.916	20992	4750	0.084
7	15.196	23935805	2248236	95.487
8	15.432	464510	78729	1.853
9	15.619	381232	52934	1.521
10	15.839	39691	8778	0.158
11	16.347	2783	606	0.011
12	16.605	2402	534	0.010
13	16.969	40036	7284	0.160
14	17.374	4613	831	0.018
15	18.835	55394	7042	0.221
Total		25067146	2426675	100.000