

Sample Name ; OVA Peptide (257-264)  
 Cat No. : RP10611  
 Lot No. : E3731020B  
 Time Processed :12:45:34  
 Month-Day-Year Processed :02/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : AlltimaTM C18 4.6 x 250 mm  
 Equipment:ZJ19010141

<Chromatogram>

mV

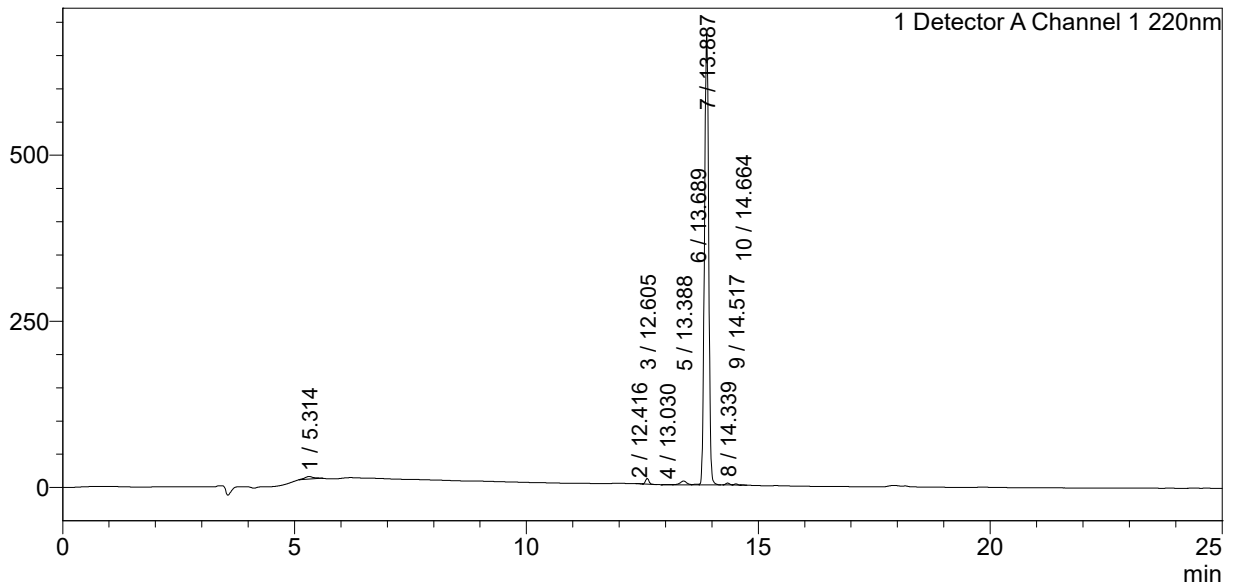

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.314	52621	3876	1.174
2	12.416	1350	264	0.030
3	12.605	46501	8727	1.037
4	13.030	3225	373	0.072
5	13.388	55422	5619	1.236
6	13.689	7778	1100	0.173
7	13.887	4290760	678508	95.713
8	14.339	15691	2829	0.350
9	14.517	8447	1617	0.188
10	14.664	1147	305	0.026
Total		4482942	703219	100.000