


Mass Spectrum

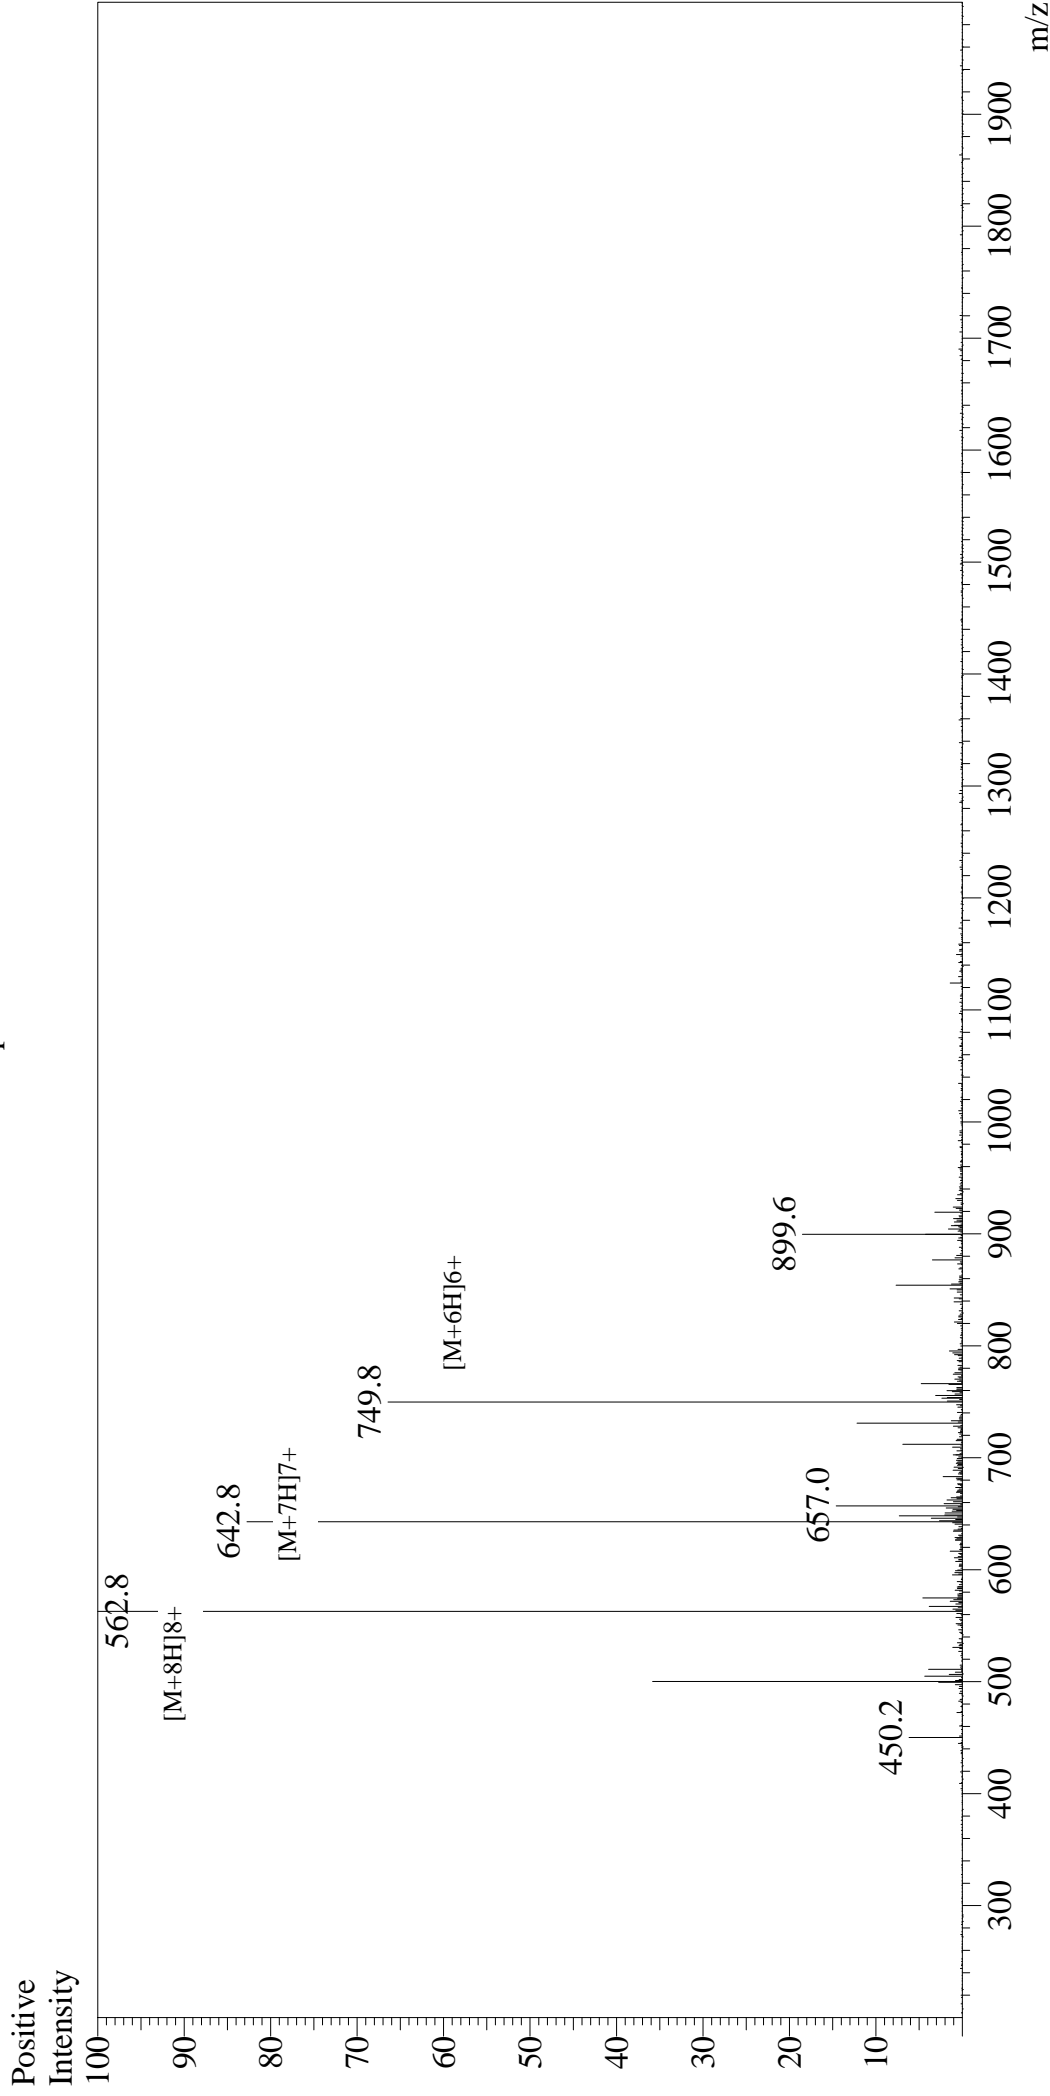

Sample Information

User : Gary
 Month-Day Processed : 03/27/20
 Time Processed : 12:34:13
 Injection Volume : 0.3
 Sample Name : LL37 (Human)
 Cat No. : RP13323
 Lot No. : E6429320C
 Theoretical MW : 4493.28
 Observed MW : 4494.4

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2ml/min
 B.conc : 50%H2O/50%MeOH