

Sample Name :FliC,Serotype a (427-441) S.paratyphi A  
 Cat. No. : RP20500  
 Lot. No. : E4975019I  
 Time Processed :14:22:59  
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

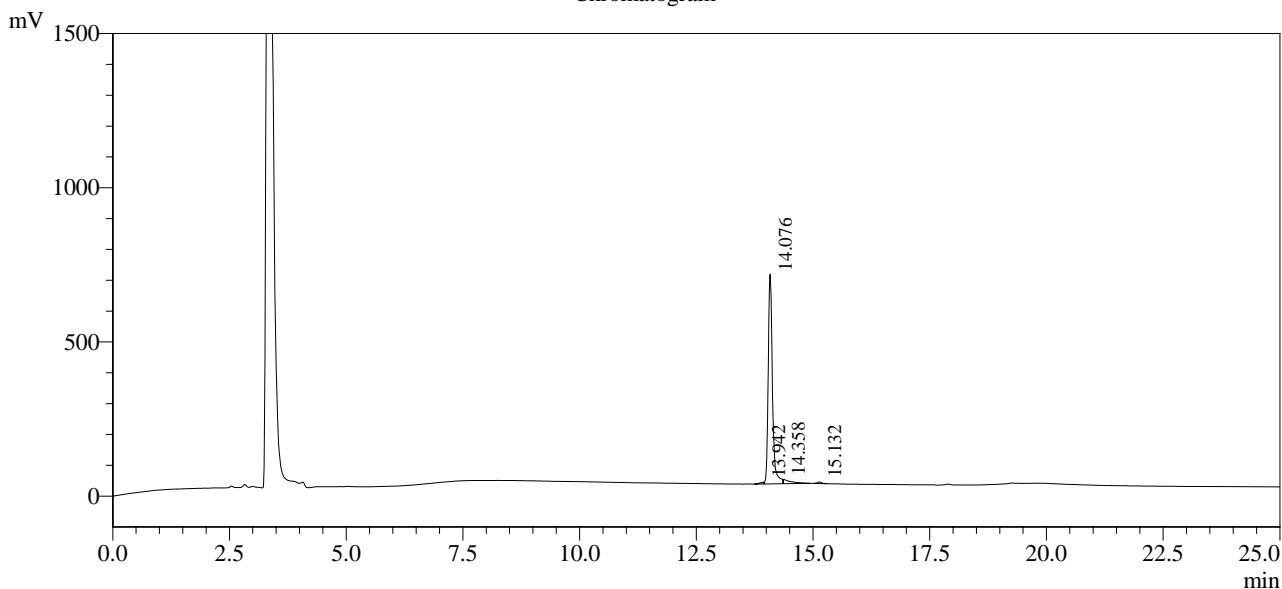

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.942	33056	5300	0.736
2	14.076	4269413	680607	95.089
3	14.358	158156	14138	3.522
4	15.132	29306	4883	0.653
Total		4489932	704927	100.000