

Sample Name :PA (224-233), Influenza  
 Cat No.:RP19991  
 Lot No.:E48306191  
 Time Processed :7:08:08  
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

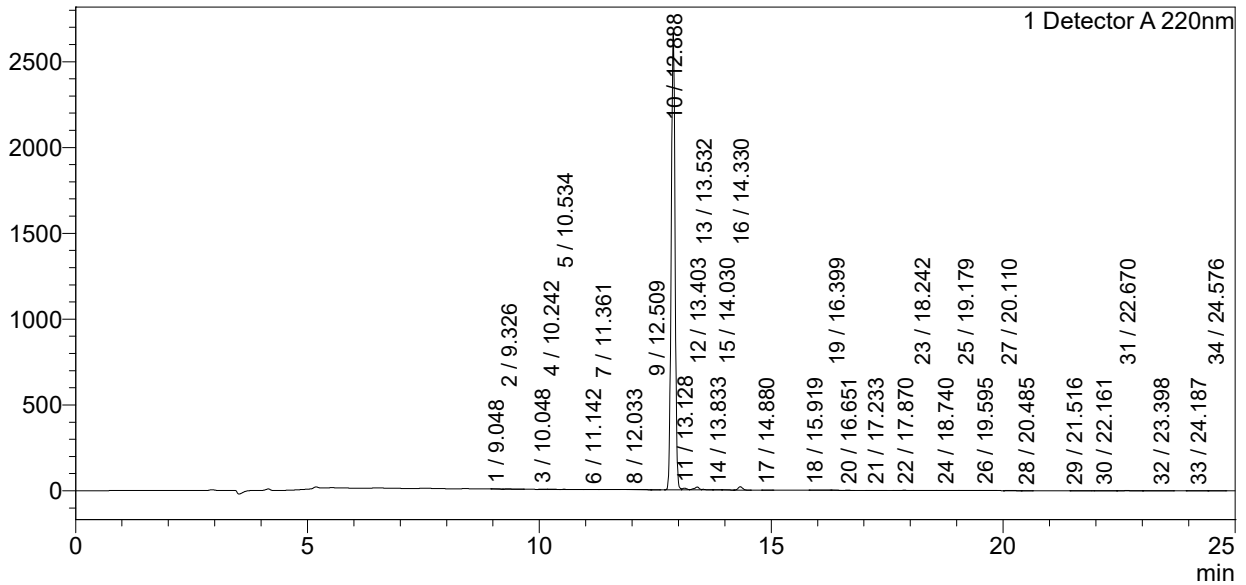

### <Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.048	1779	245	0.011
2	9.326	8205	473	0.052
3	10.048	6566	640	0.041
4	10.242	11308	684	0.071
5	10.534	16544	1006	0.104
6	11.142	8013	608	0.050
7	11.361	11273	1203	0.071
8	12.033	15167	1229	0.095
9	12.509	2472	391	0.016
10	12.888	15425364	2662126	96.826
11	13.128	65630	10481	0.412
12	13.403	129665	16988	0.814
13	13.532	18725	3587	0.118
14	13.833	2898	588	0.018
15	14.030	1835	234	0.012

Peak#	Ret. Time	Area	Height	Area%
16	14.330	127428	19359	0.800
17	14.880	1789	249	0.011
18	15.919	7182	1044	0.045
19	16.399	1186	145	0.007
20	16.651	6163	1065	0.039
21	17.233	4018	292	0.025
22	17.870	12279	1269	0.077
23	18.242	4970	297	0.031
24	18.740	3592	285	0.023
25	19.179	2633	208	0.017
26	19.595	1231	166	0.008
27	20.110	5451	507	0.034
28	20.485	1142	161	0.007
29	21.516	1175	56	0.007
30	22.161	2821	205	0.018
31	22.670	14357	1469	0.090
32	23.398	3846	194	0.024
33	24.187	2353	169	0.015
34	24.576	1928	163	0.012
Total		15930989	2727787	100.000