

Sample Name :Abz-FR-K (Dnp)-P-OH
 Cat. No. : RP20115
 Lot. No. : E4830319I
 Time Processed : 23:59:53
 Month-Day-Year Processed : 10/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

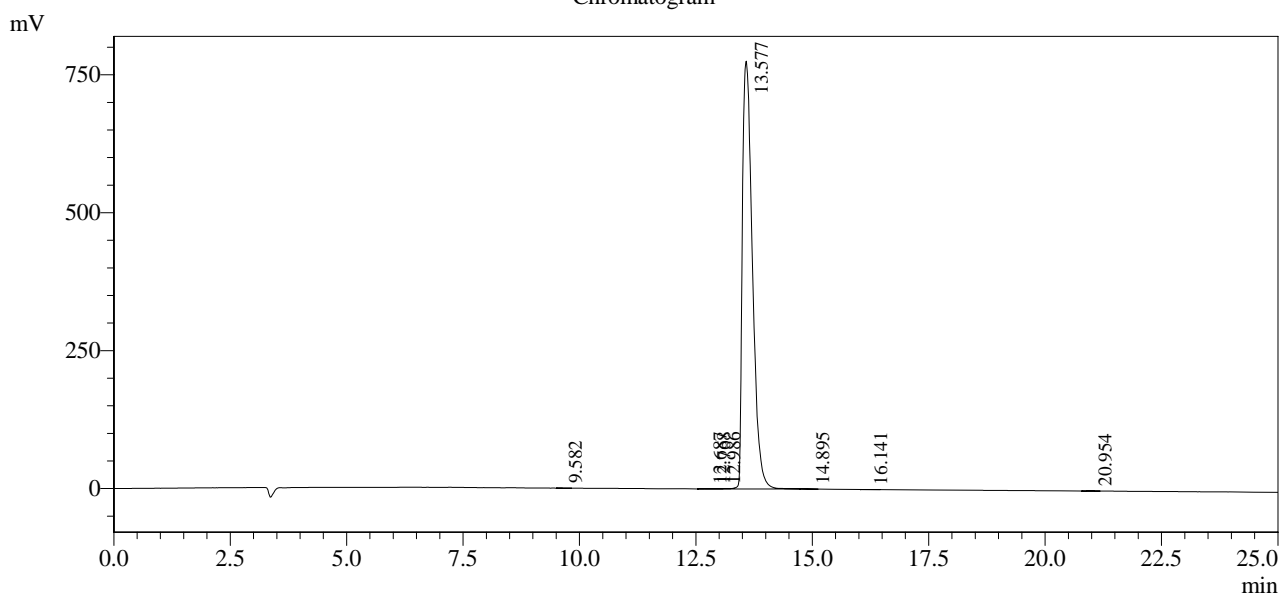

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.582	1226	80	0.011
2	12.687	2232	331	0.019
3	12.768	2313	298	0.020
4	12.986	1684	261	0.014
5	13.577	11656906	775364	99.825
6	14.895	4871	526	0.042
7	16.141	4860	470	0.042
8	20.954	3197	336	0.027
Total		11677289	777666	100.000