

Sample Name : Autocamtide 2
 Cat. No. : RP10271
 Lot. No. : E4707319I
 Time Processed : 11:12:10
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

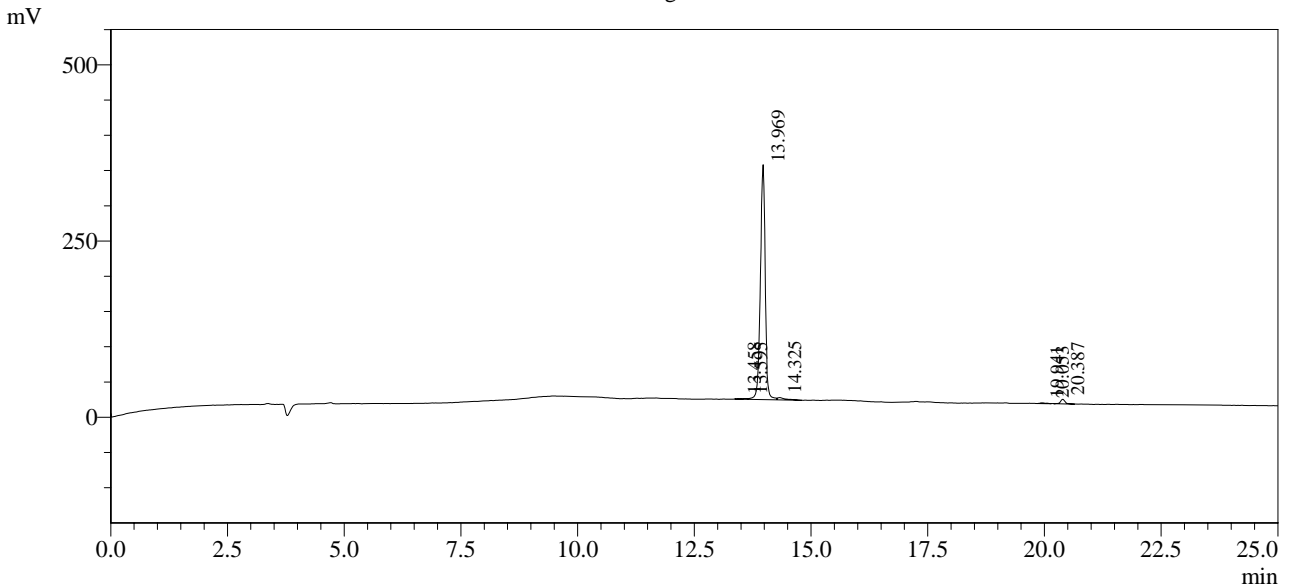

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.458	1909	381	0.075
2	13.595	7032	1006	0.278
3	13.969	2428098	333192	95.911
4	14.325	40776	3176	1.611
5	19.941	6588	1024	0.260
6	20.053	2042	541	0.081
7	20.387	45184	6528	1.785
Total		2531629	345847	100.000