


Mass Spectrum

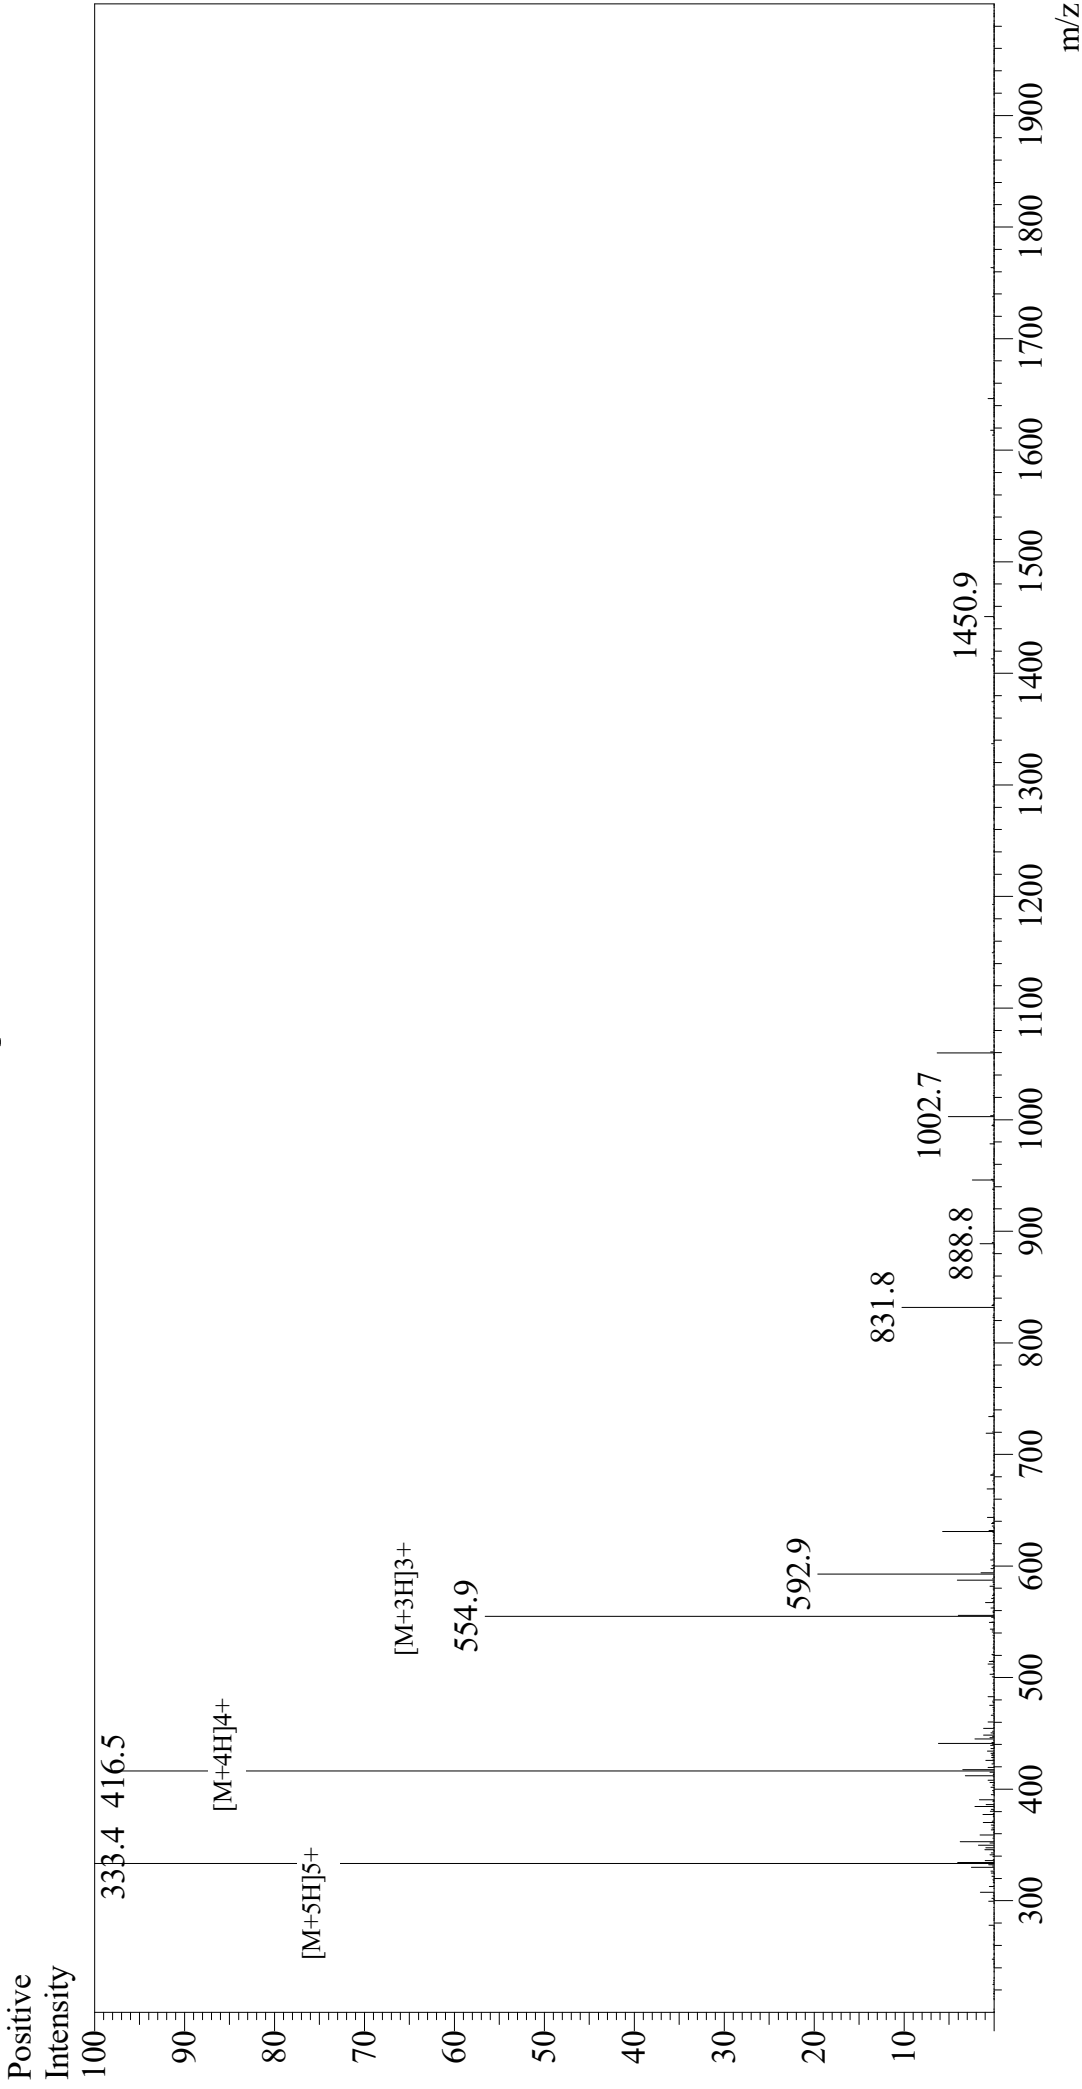

Sample Information
Month-Day Processed : 09/10/20
Time Processed : 04:42:46 PM
Injection Volume : 0.4
Sample Name : Cys-TAT(47-57)
Cat No.: RP20343
Lot No.: E6893820H
Theoretical MW : 1661.99
Observed MW : 1662.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH