


Mass Spectrum

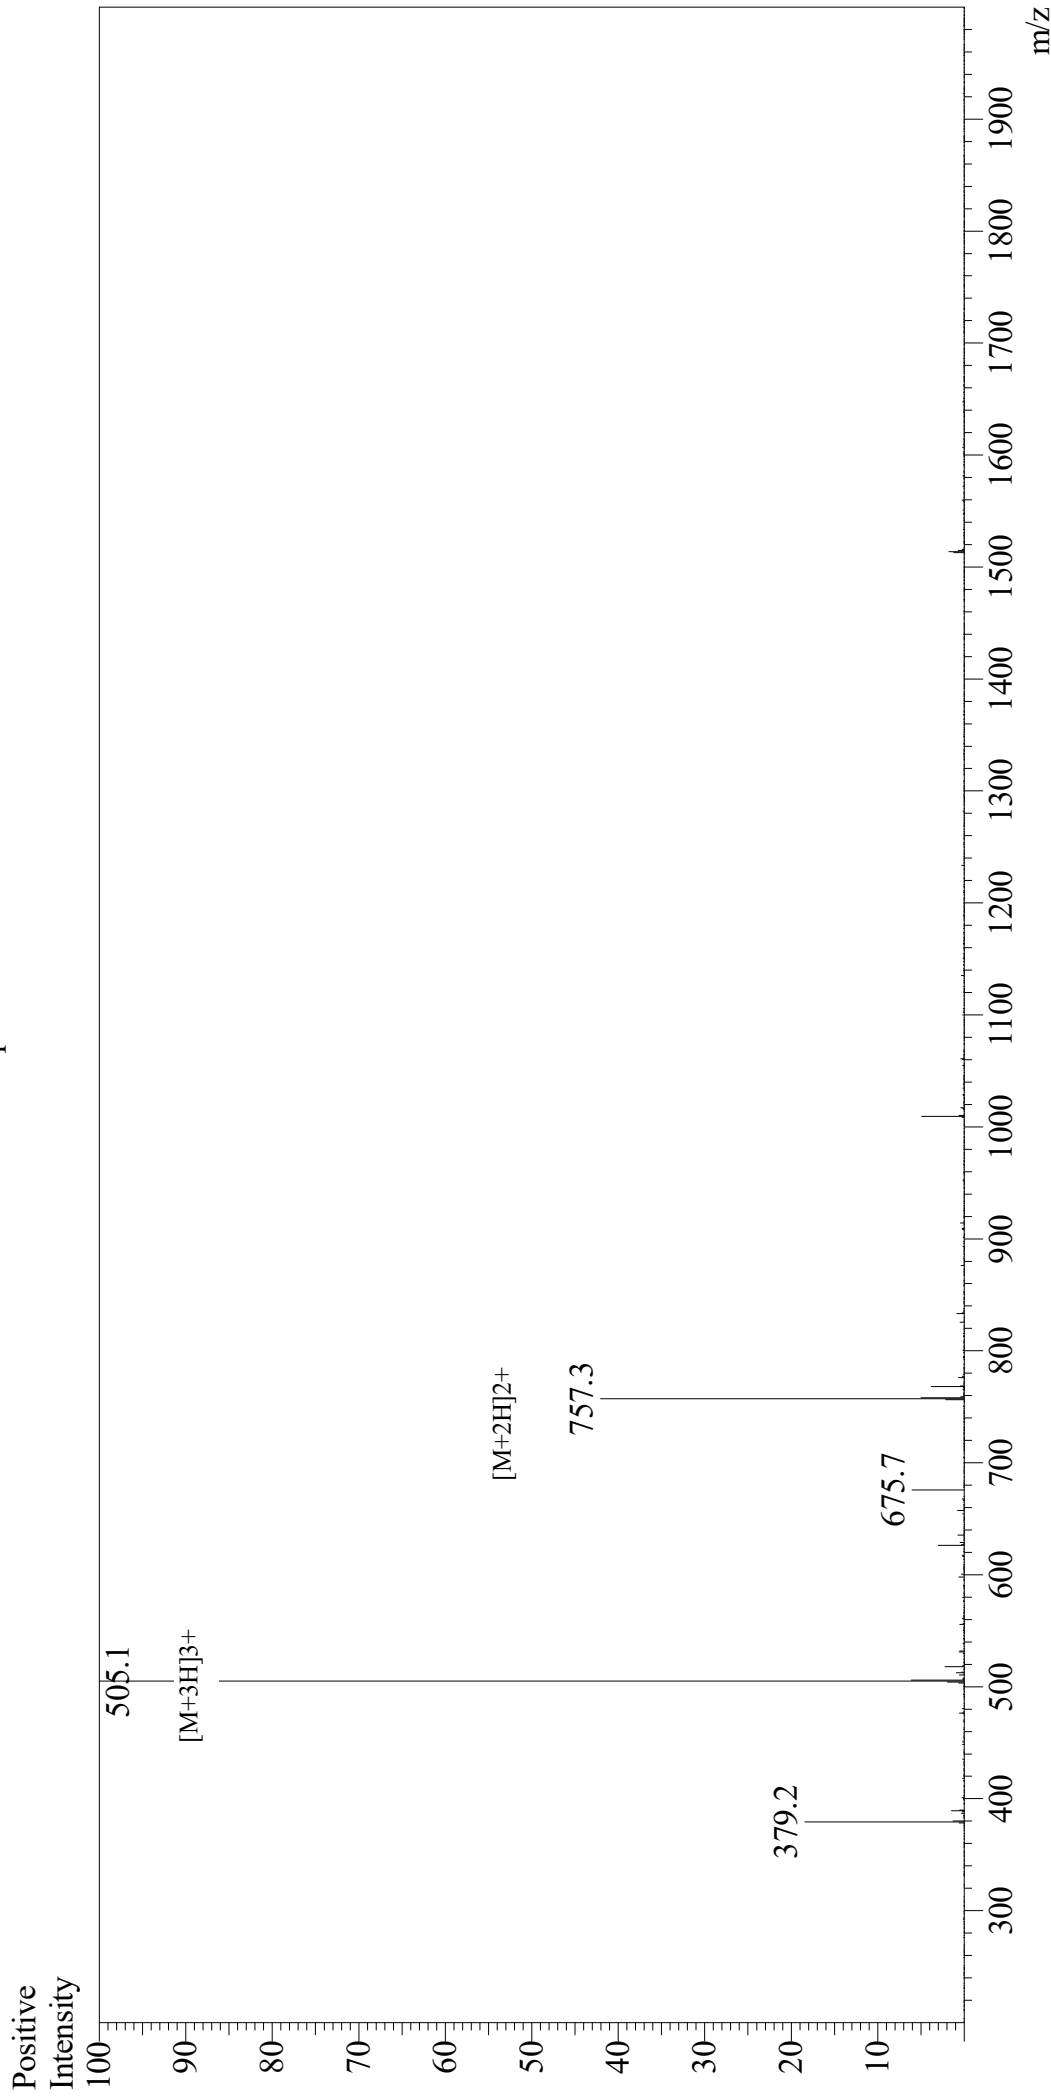

Sample Information

User : Gary
Month-Day Processed : 10/03/19
Time Processed : 09:56:35 AM
Injection Volume : 0.3
Sample Name : γ -1-Melanocyte Stimulating Hormone (MSH), amide
Cat No. : RP10650
Lot No. : E9298819I
Theoretical MW : 1512.90
Observed MW : 1512.3

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH