

Sample Name : HIV-1 TAT (48-60)  
 Cat. No. : RP20423  
 Lot. No. : E5572919J  
 Time Processed :7:08:51  
 Month-Day-Year Processed :10/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

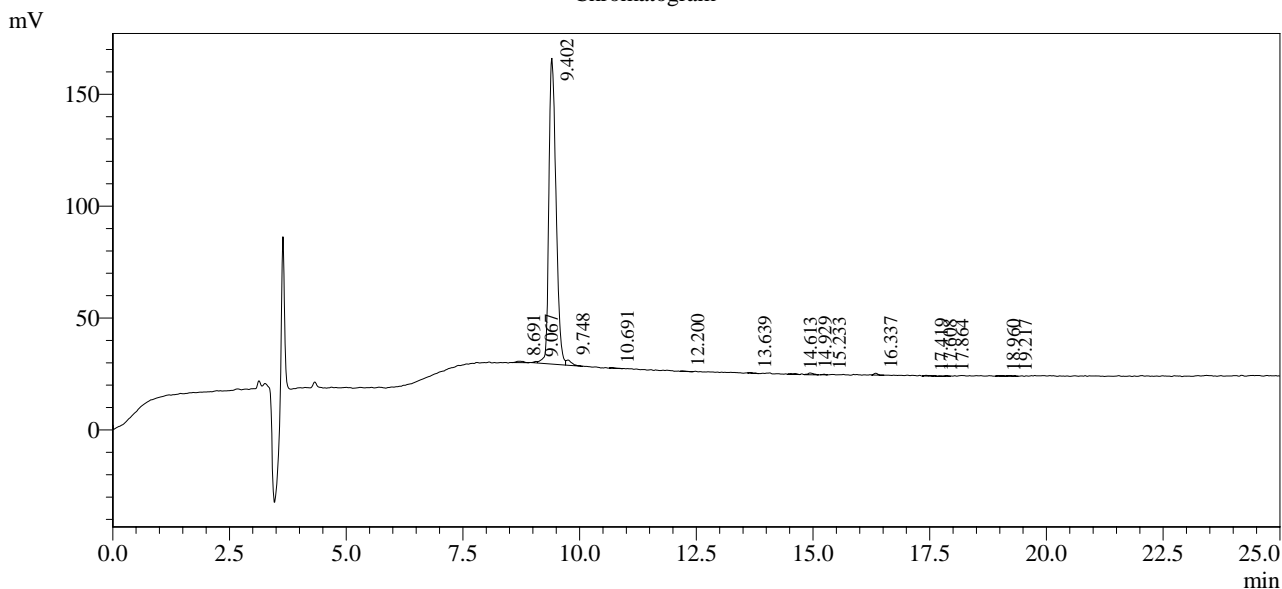

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.691	6926	626	0.457
2	9.067	3435	650	0.227
3	9.402	1454028	136668	95.969
4	9.748	19508	2323	1.288
5	10.691	2239	315	0.148
6	12.200	1830	273	0.121
7	13.639	1505	232	0.099
8	14.613	3084	349	0.204
9	14.929	6646	766	0.439
10	15.233	1152	295	0.076
11	16.337	4740	840	0.313
12	17.419	2986	320	0.197
13	17.608	1046	268	0.069
14	17.864	1809	257	0.119
15	18.960	1678	201	0.111
16	19.217	2497	254	0.165
Total		1515109	144638	100.000