

Sample Name :Endothelin 1, human, porcine
 Cat No. :RP12758
 Lot No. :E6260020I
 Time Processed :9:29:40 AM
 Month-Day-Year Processed :09/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

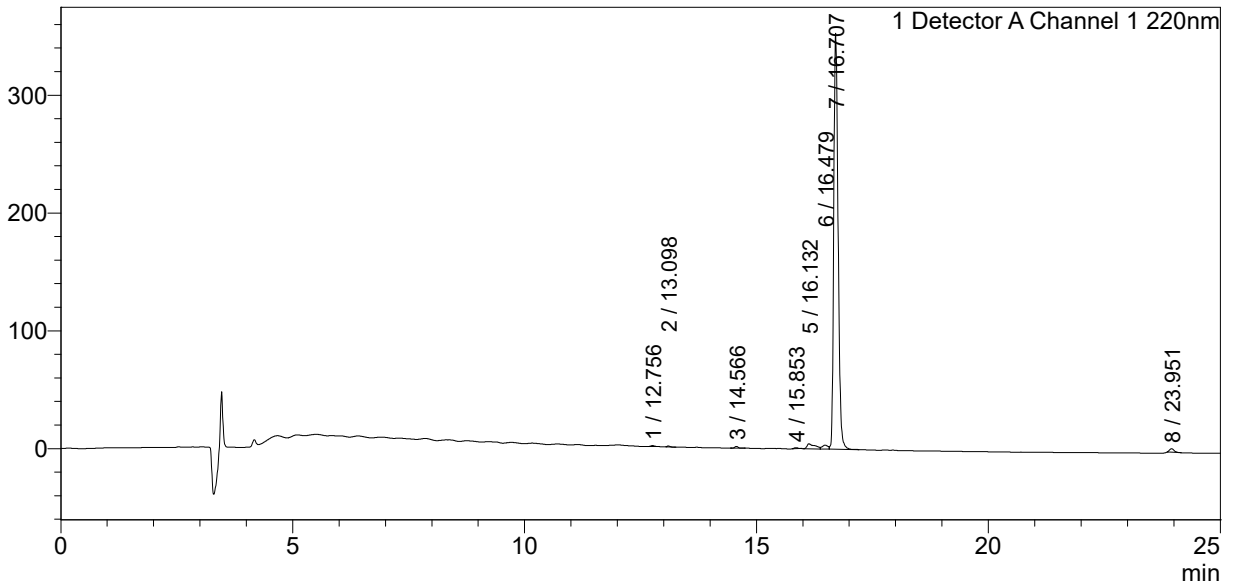

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.756	4406	812	0.181
2	13.098	2223	679	0.092
3	14.566	6576	1442	0.271
4	15.853	4706	870	0.194
5	16.132	50278	4214	2.070
6	16.479	28383	3344	1.169
7	16.707	2312458	353232	95.206
8	23.951	19867	2921	0.818
Total		2428896	367515	100.000