

Sample Name :Bombesin  
 Cat No. :RP11157  
 Lot No. : PE4301902  
 Time Processed :9:01:35  
 Month-Day-Year Processed :02/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010508

<Chromatogram>

mV

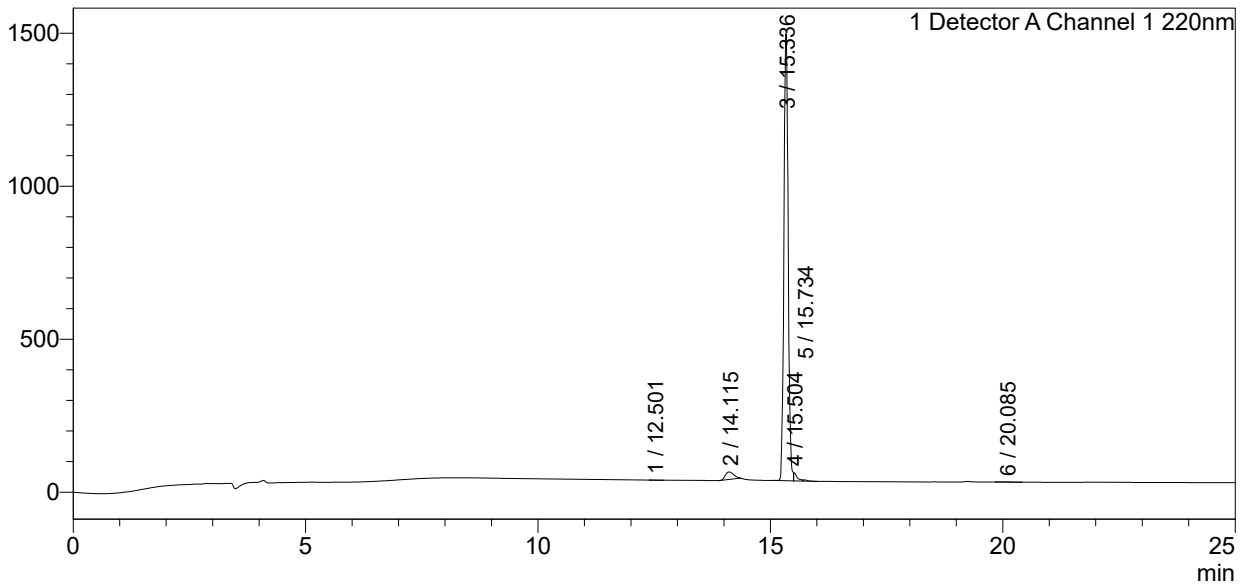

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.501	5216	794	0.054
2	14.115	306880	24581	3.161
3	15.336	9237540	1460501	95.154
4	15.504	129486	27156	1.334
5	15.734	23638	3957	0.243
6	20.085	5246	541	0.054
Total		9708006	1517530	100.000