

Sample Name : SAMs Peptide
 Cat. No. : RP10172
 Lot. No. : PE4861611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

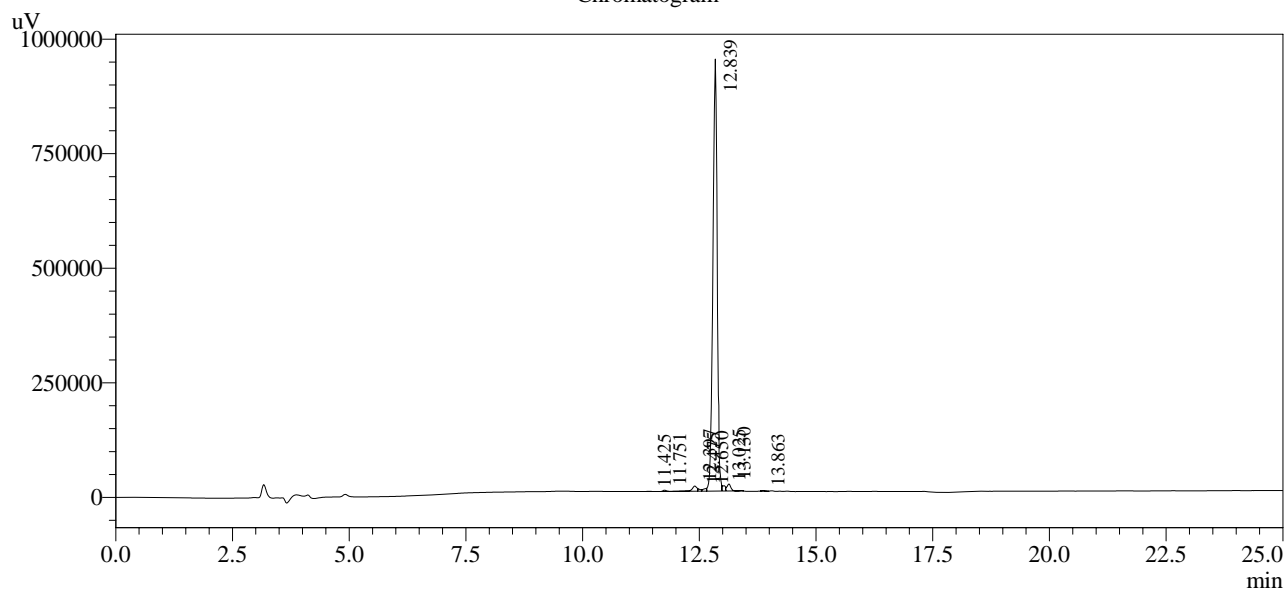

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.425	3148	385	0.050
2	11.751	16781	2852	0.265
3	12.397	92364	11517	1.459
4	12.475	19886	5298	0.314
5	12.650	31678	6091	0.500
6	12.839	6022001	942967	95.109
7	13.025	53470	11495	0.844
8	13.130	86397	15186	1.365
9	13.863	5937	1256	0.094
Total		6331663	997049	100.000