

Sample Name : GP(33-41)
 Cat. No. : RP20091
 Lot. No. : PE3131704

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

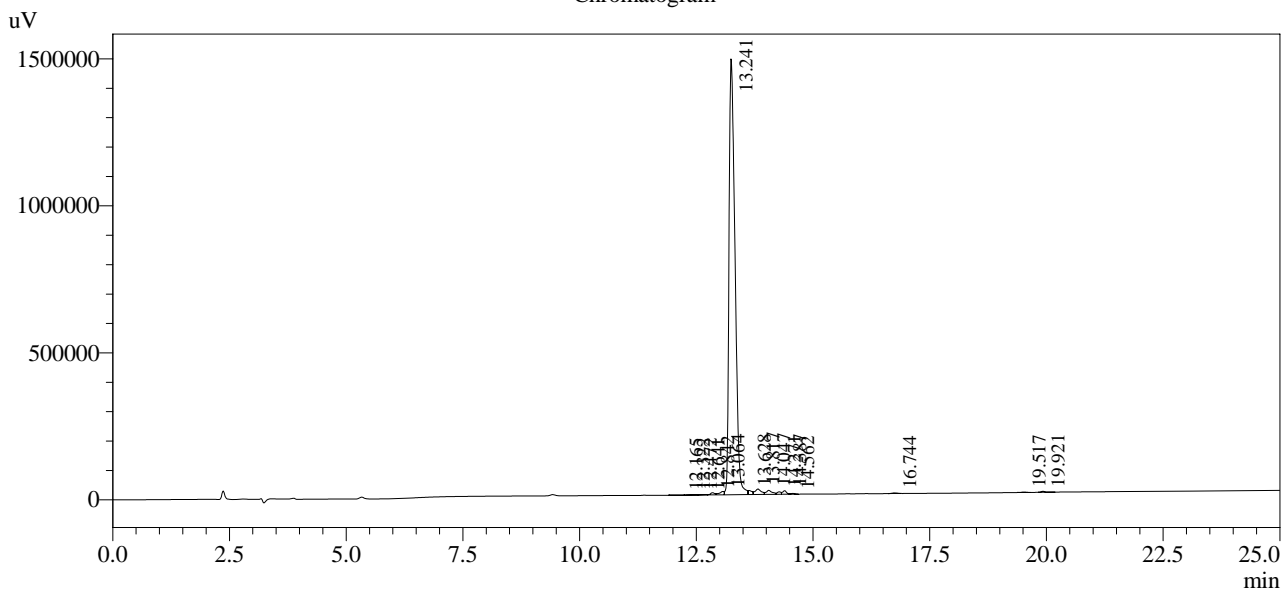

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.165	1949	197	0.014
2	12.322	1680	355	0.012
3	12.472	3063	563	0.022
4	12.641	7492	1018	0.054
5	12.842	44977	7394	0.324
6	13.064	80456	11395	0.579
7	13.241	13216094	1482561	95.104
8	13.628	76155	13666	0.548
9	13.817	173129	18797	1.246
10	14.047	123262	13816	0.887
11	14.271	47837	8621	0.344
12	14.387	67899	11970	0.489
13	14.562	13474	2553	0.097
14	16.744	13660	1968	0.098
15	19.517	8578	1333	0.062
16	19.921	16737	3354	0.120
Total		13896442	1579561	100.000