

Sample Name : AMARA peptide
 Cat. No. : RP20472
 Lot. No. : PE8021810
 Time Processed :9:36:43
 Month-Day-Year Processed :10/21/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

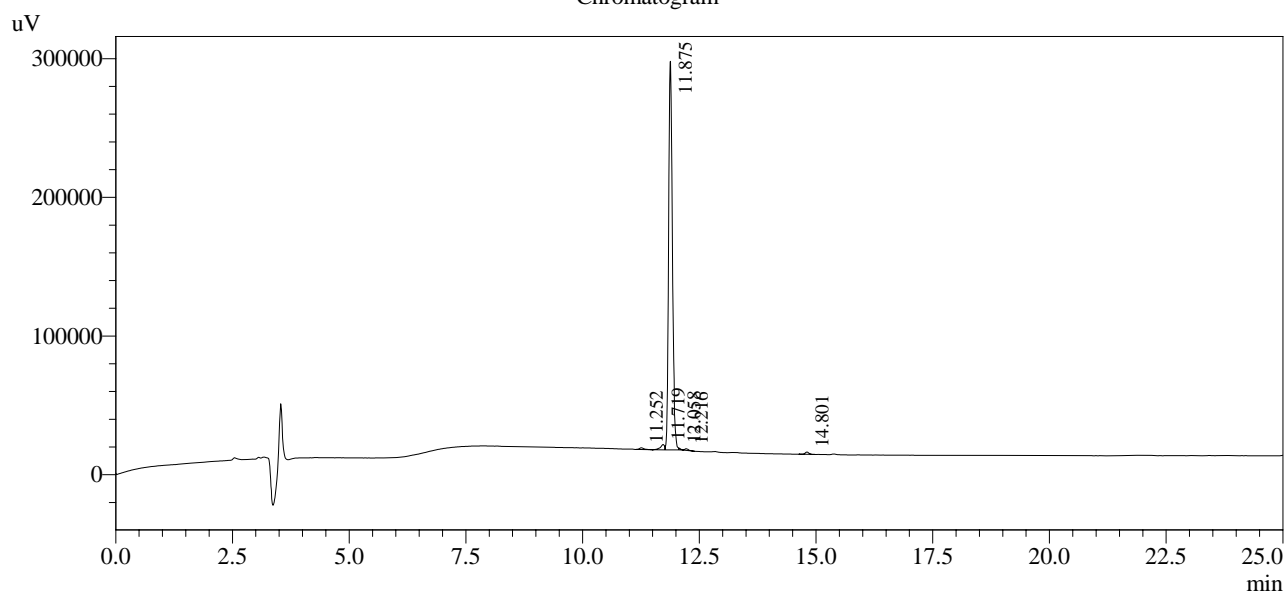

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.252	8389	1228	0.512
2	11.719	24348	3807	1.487
3	11.875	1585975	279838	96.872
4	12.058	3105	1412	0.190
5	12.216	5947	1115	0.363
6	14.801	9430	1663	0.576
Total		1637193	289061	100.000