

Sample Name : Crustacean Cardioactive Peptide (CCAP)  
 Cat. No. : RP10572  
 Lot. No. : PE2001702

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

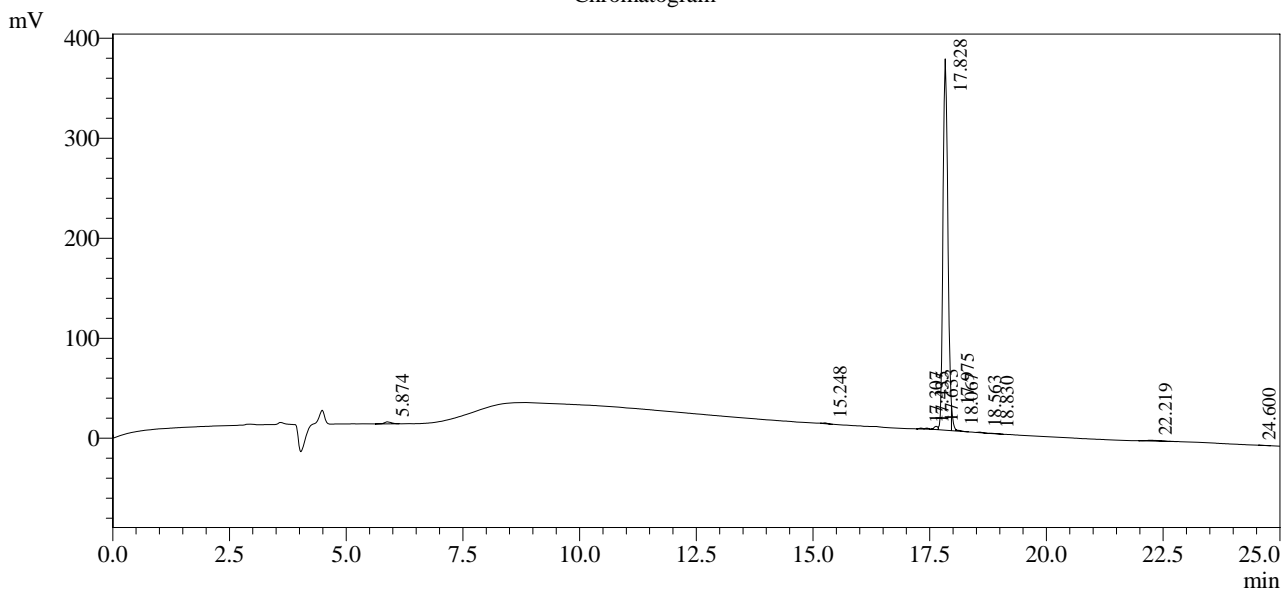

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.874	19572	1918	0.688
2	15.248	5043	794	0.177
3	17.307	5363	894	0.189
4	17.435	5848	1043	0.206
5	17.633	18919	3253	0.665
6	17.828	2713840	371376	95.386
7	17.975	43496	20480	1.529
8	18.067	6962	1305	0.245
9	18.563	3447	534	0.121
10	18.830	3242	291	0.114
11	22.219	17367	699	0.610
12	24.600	2013	200	0.071
Total		2845110	402785	100.000