

Sample Name :Neuropeptide Y, human
 Cat No :RP10492
 Lot No :E7755121B
 Time Processed :10:26:55 PM
 Month-Day-Year Processed :02/05/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

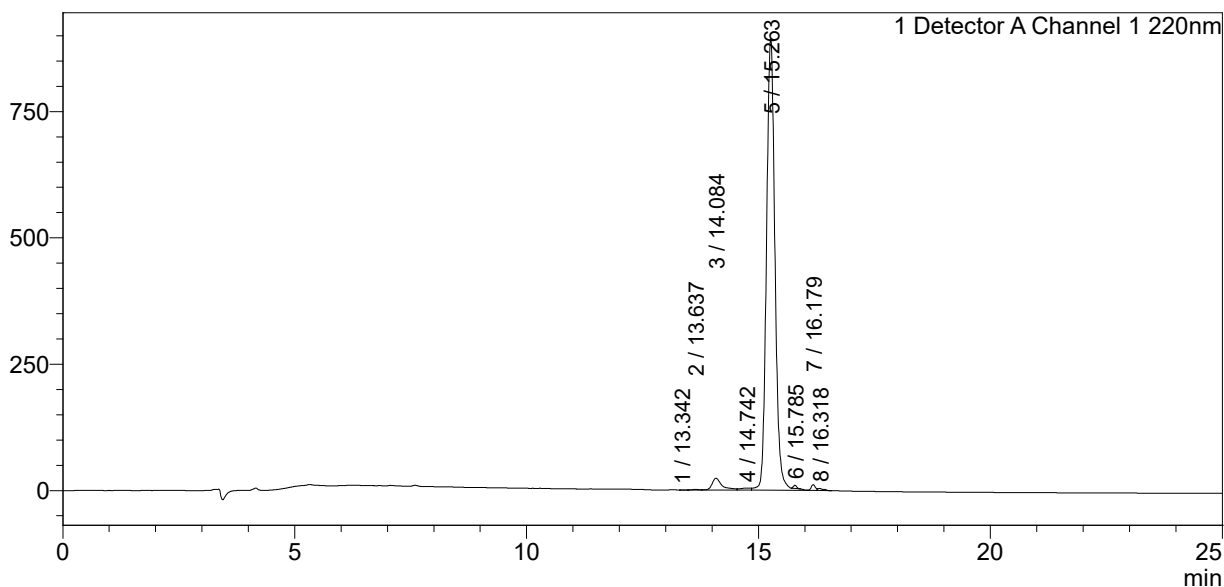

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.342	245	47	0.002
2	13.637	11486	1095	0.097
3	14.084	350217	23416	2.945
4	14.742	65128	4073	0.548
5	15.263	11328874	893610	95.267
6	15.785	30776	6292	0.259
7	16.179	68412	11377	0.575
8	16.318	36550	4248	0.307
Total		11891688	944158	100.000