

Sample Name : β -Amyloid (1-42), human
 Cat No. :RP20527
 Lot No. :E0976919K
 Time Processed : 9:54:29
 Month-Day-Year Processed : 12/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

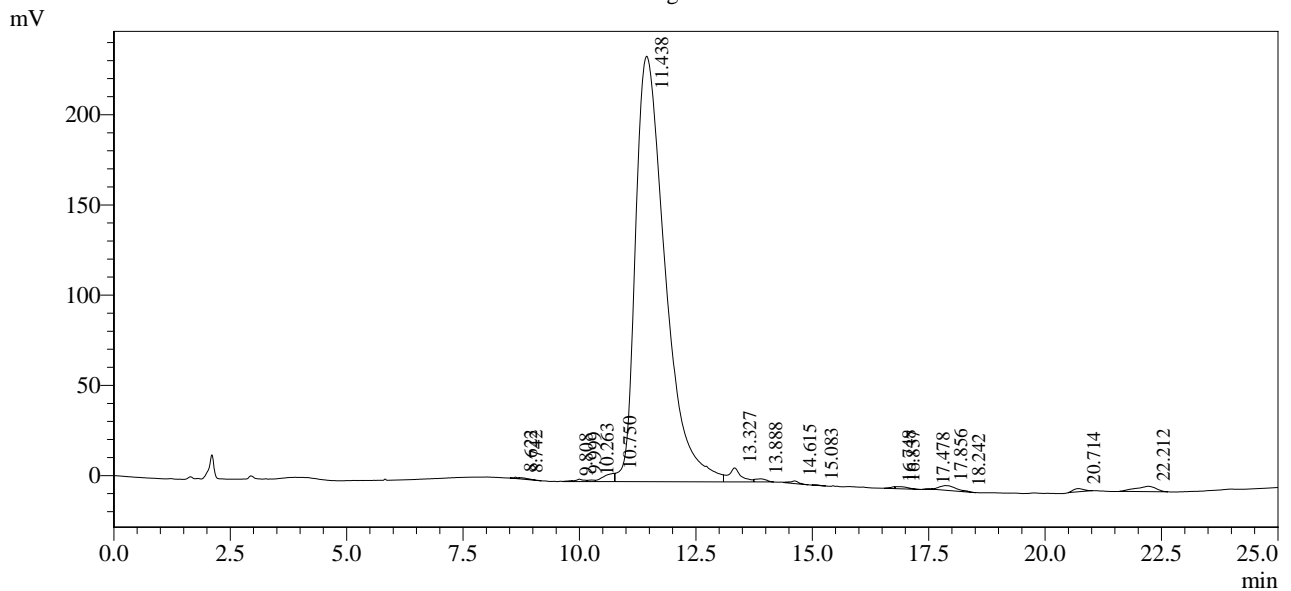

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.622	4655	753	0.043
2	8.742	10093	669	0.092
3	9.808	3619	450	0.033
4	9.999	15851	1377	0.145
5	10.263	8781	900	0.080
6	10.750	73840	4593	0.674
7	11.438	10427471	235804	95.209
8	13.327	144614	7738	1.320
9	13.888	27418	1692	0.250
10	14.615	18810	1446	0.172
11	15.083	2229	320	0.020
12	16.748	7560	1072	0.069
13	16.837	21844	1173	0.199
14	17.478	1061	154	0.010
15	17.856	61769	2552	0.564
16	18.242	4710	635	0.043
17	20.714	28233	1744	0.258
18	22.212	89641	2948	0.818
Total		10952196	266020	100.000