

Sample Name : OVA G4 peptide
 Cat. No. : RP20398 Lot. No. : PE4731810
 Time Processed : 15:50:52
 Month-Day-Year Processed : 11/04/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment: ZJ17010507

<Chromatogram>

mV

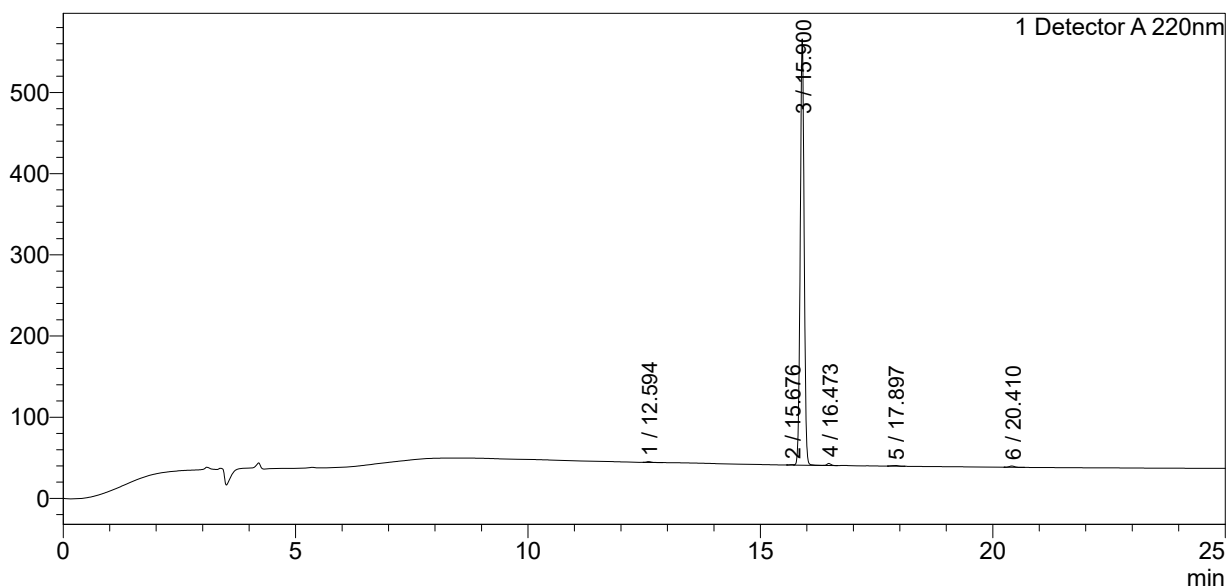

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.594	6902	1023	0.221
2	15.676	2799	518	0.090
3	15.900	3076005	525002	98.556
4	16.473	14457	2493	0.463
5	17.897	8026	955	0.257
6	20.410	12900	1623	0.413
Total		3121088	531614	100.000