

Sample Name :Atrial Natriuretic Peptide (ANP) (1-28), rat
 Cat No.: RP11195
 Lot No.: E3677620G
 Time Processed :9:47:31
 Month-Day-Year Processed :07/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	95
35.10	Pumps	Pump A B.Conc	5
40.20	Pumps	Pump A B.Conc	5
41.09	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

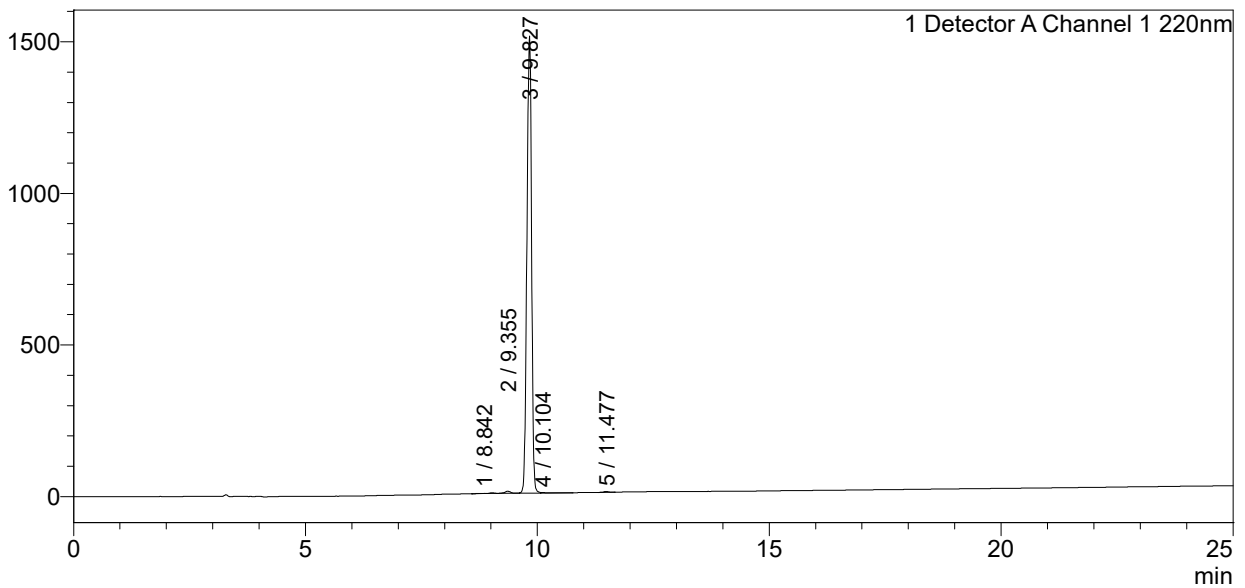

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.842	762	8	0.007
2	9.355	76499	6741	0.723
3	9.827	10475490	1508283	98.968
4	10.104	14846	1603	0.140
5	11.477	17087	2827	0.161
Total		10584684	1519462	100.000