

Sample Name: IRBP (1-20), human  
 Cat. No. : RP20269  
 Lot. No. : E7072719K  
 Time Processed: 12:03:07 PM  
 Month-Day-Year Processed : 11/29/2019  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm  
 Equipment: ZJ19010325

### <Chromatogram>

mV

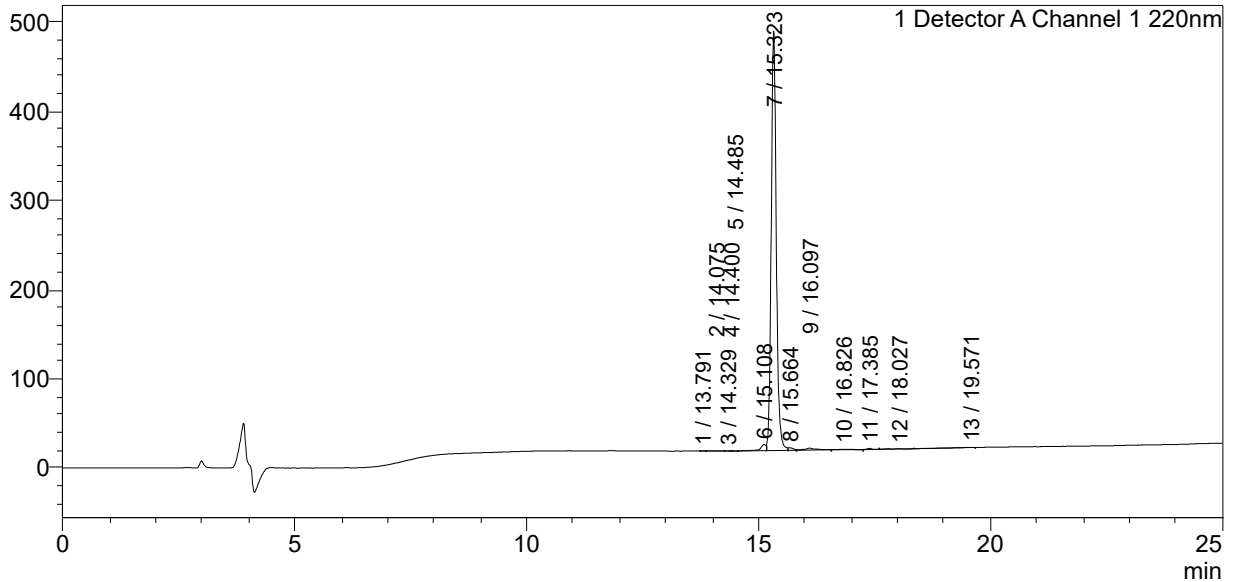

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.791	267	64	0.007
2	14.075	2107	209	0.057
3	14.329	304	70	0.008
4	14.400	171	47	0.005
5	14.485	102	41	0.003
6	15.108	48404	6626	1.299
7	15.323	3589305	470622	96.300
8	15.664	19530	2778	0.524
9	16.097	35261	2113	0.946
10	16.826	7674	422	0.206
11	17.385	9199	1405	0.247
12	18.027	9053	463	0.243
13	19.571	5827	137	0.156
Total		3727204	484995	100.000