

Sample Name :W Peptide, WKYVMm  
 Cat No. :RP20299  
 Lot No. :E2344520A  
 Time Processed :16:25:03  
 Month-Day-Year Processed :01/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

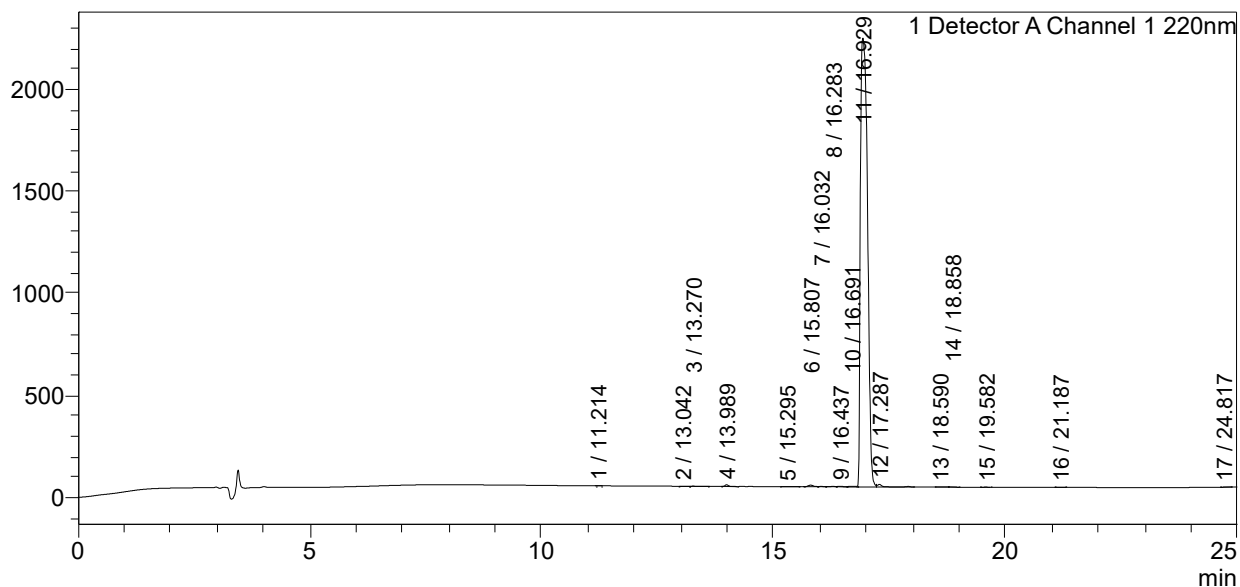

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.214	2005	519	0.008
2	13.042	3491	306	0.015
3	13.270	10550	736	0.044
4	13.989	47993	8524	0.202
5	15.295	7494	756	0.032
6	15.807	63307	7685	0.266
7	16.032	11000	1449	0.046
8	16.283	15829	1650	0.067
9	16.437	23922	2384	0.101
10	16.691	30493	3257	0.128
11	16.929	23442315	2201755	98.576
12	17.287	101118	12449	0.425
13	18.590	9732	1330	0.041
14	18.858	3591	480	0.015
15	19.582	2241	451	0.009

Peak#	Ret. Time	Area	Height	Area%
16	21.187	3964	698	0.017
17	24.817	1909	191	0.008
Total		23780953	2244621	100.000