

Sample Name : [Arg<sup>8</sup>]-Vasotocin  
 Cat. No. : RP10061 □ □ Lot. No. : PE6351811  
 Time Processed : 20:28:04  
 Month-Day-Year Processed : 11/27/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

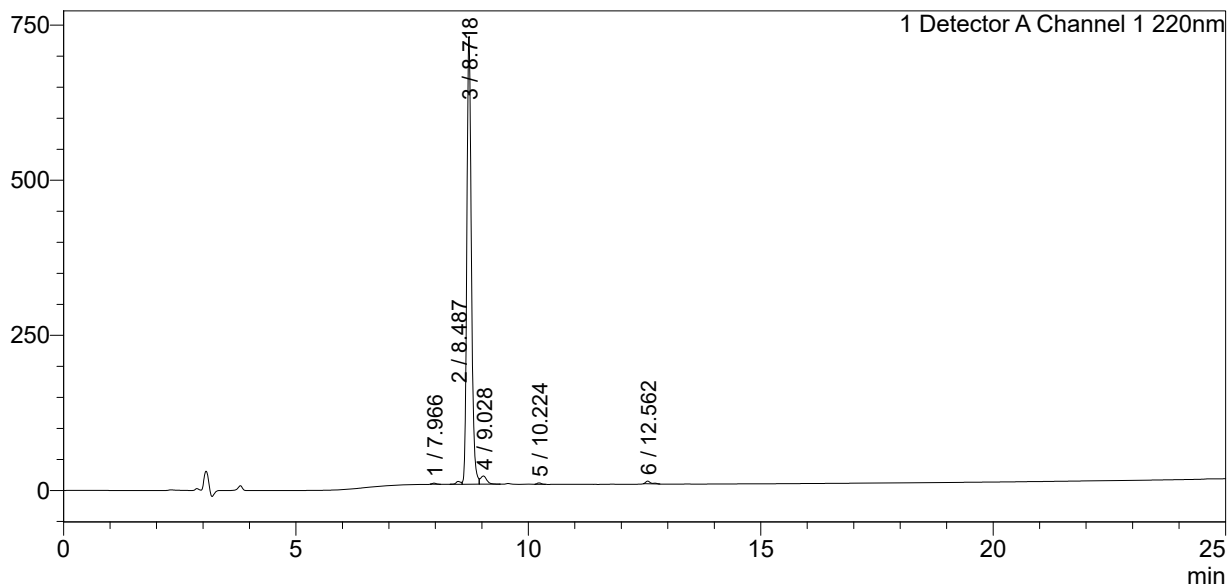

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.966	10334	1781	0.202
2	8.487	33682	4556	0.659
3	8.718	4894014	721589	95.786
4	9.028	123442	13285	2.416
5	10.224	13605	2305	0.266
6	12.562	34248	4318	0.670
Total		5109325	747833	100.000