

Sample Name : HIV gag199-207
 Cat No. : RP20251
 Lot No. : E6129720G
 Time Processed : 8:31:18 AM
 Month-Day-Year Processed : 07/06/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

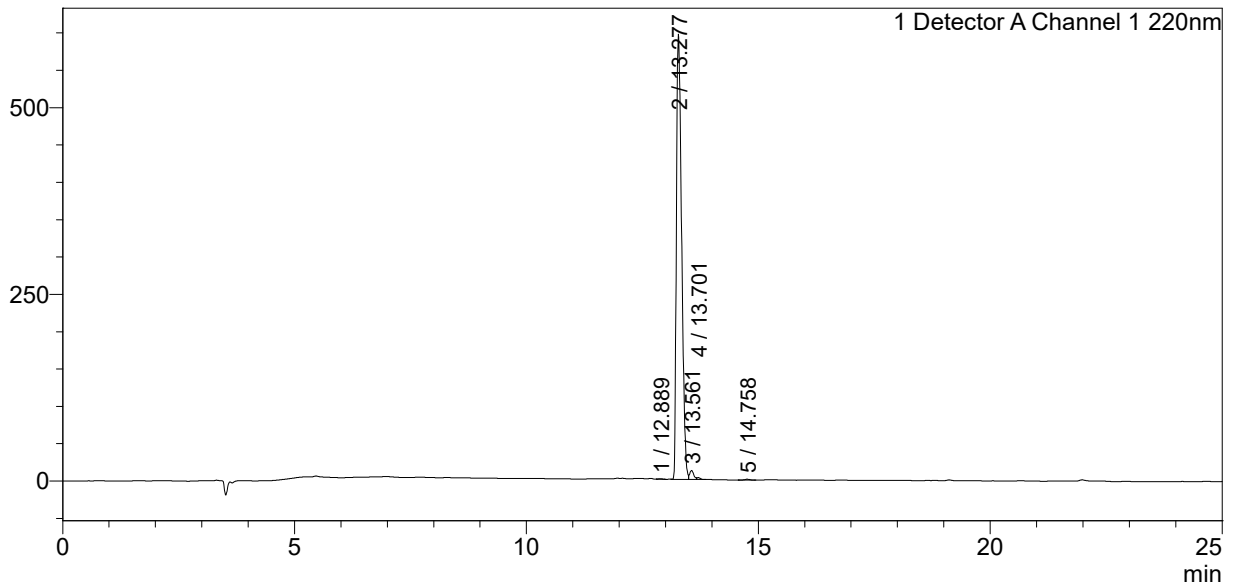

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.889	4537	831	0.095
2	13.277	4682959	596382	97.950
3	13.561	72685	12176	1.520
4	13.701	12623	2524	0.264
5	14.758	8165	1102	0.171
Total		4780969	613016	100.000