


Mass Spectrum

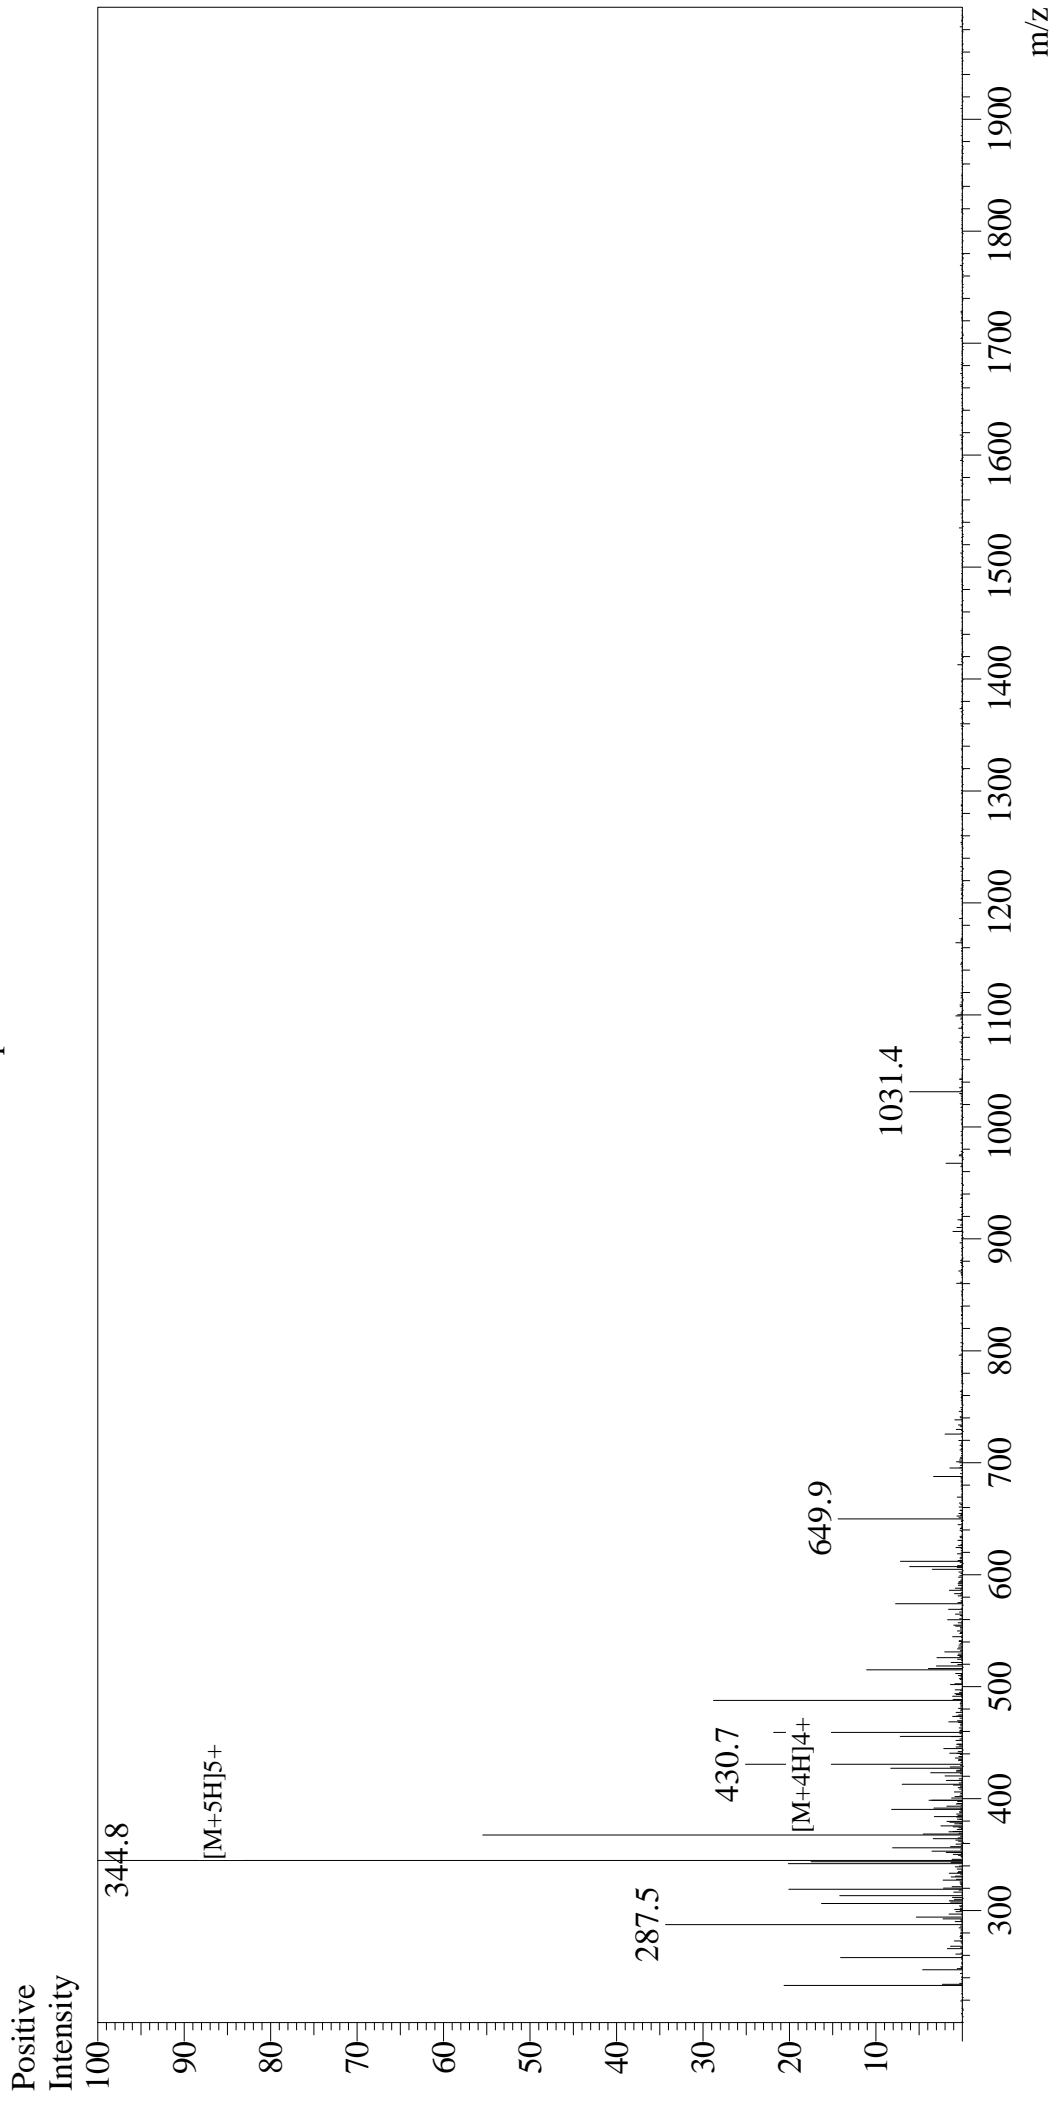

Sample Information

User : Gary
Month-Day Processed : 11/18/19
Time Processed : 13:24:43
Injection Volume : 0.3
Sample Name : HIV-1 TAT (48-60)
Cat No. : RP20423
Lot No. : E6898719K
Theoretical MW : 1719.00
Observed MW : 1719.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH