

Sample Name :Influenza HA (518-526)
 Cat No. :RP20284
 Lot No. :E4867319I
 Time Processed :2:16:38 PM
 Month-Day-Year Processed :09/21/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

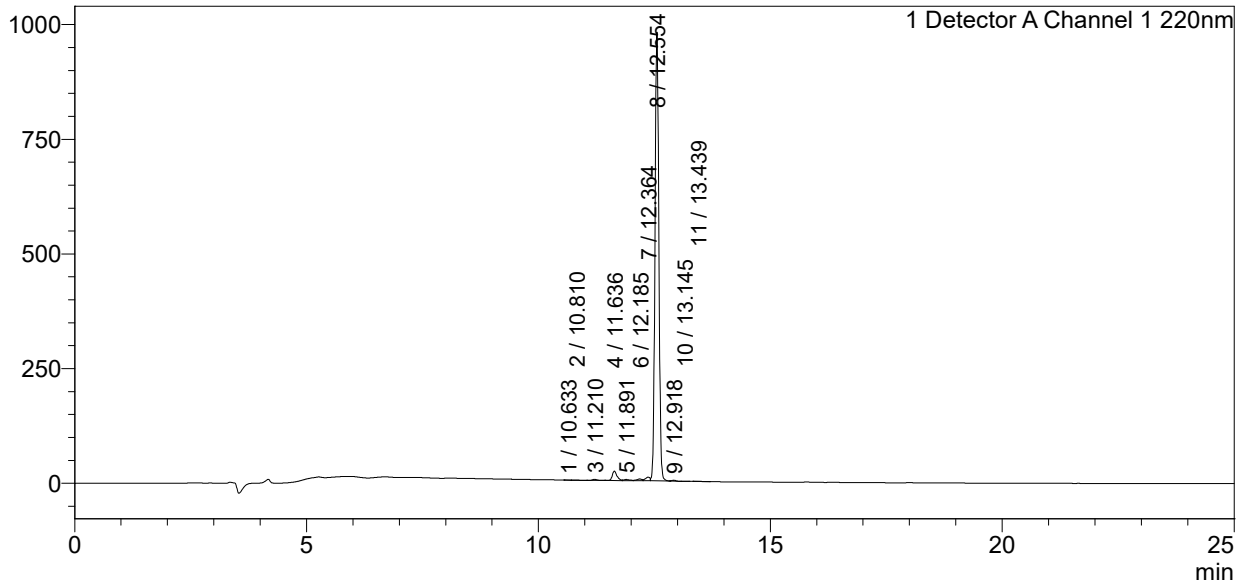

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.633	1107	152	0.019
2	10.810	5093	815	0.086
3	11.210	14798	2288	0.249
4	11.636	142877	20630	2.406
5	11.891	21215	2346	0.357
6	12.185	31205	3935	0.526
7	12.364	53978	7840	0.909
8	12.554	5651389	978570	95.182
9	12.918	10433	1960	0.176
10	13.145	1161	215	0.020
11	13.439	4183	679	0.070
Total		5937440	1019430	100.000