

Sample Name : BDC2.5 mimotope 1040-31  
Cat. No. :RP20518  
Lot. No. :E4942519I  
Time Processed :12:58:22  
Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

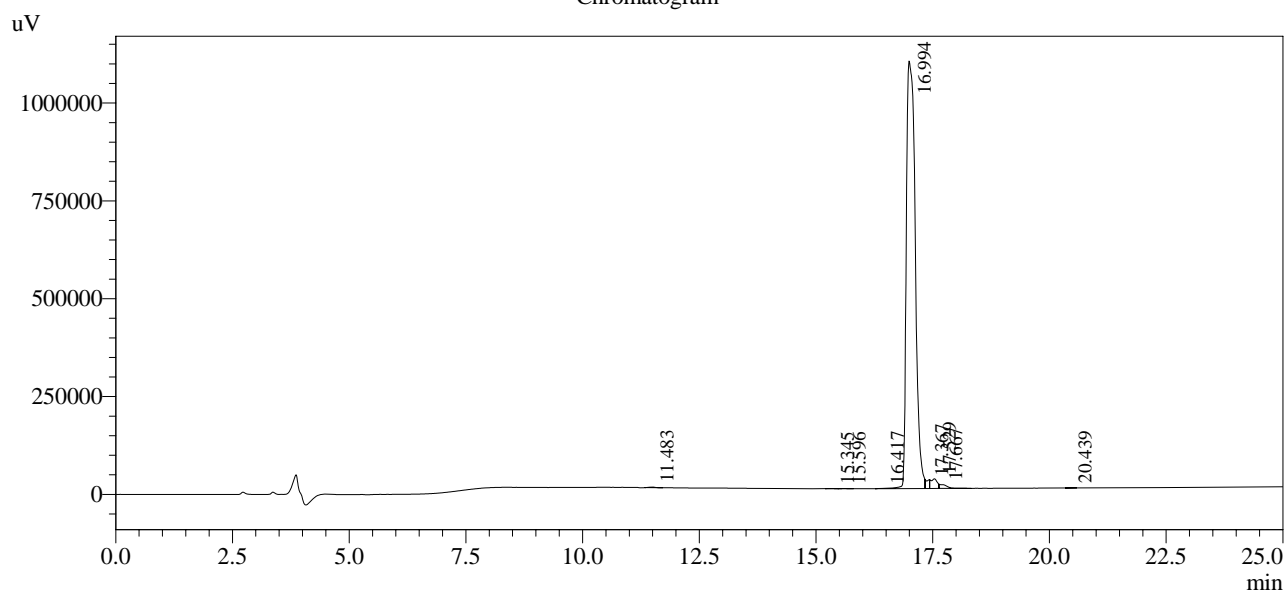

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.483	11238	1406	0.075
2	15.345	2814	456	0.019
3	15.596	2980	443	0.020
4	16.417	4284	558	0.029
5	16.994	14388358	1091877	96.645
6	17.367	124432	20367	0.836
7	17.529	236631	23798	1.589
8	17.667	114181	10004	0.767
9	20.439	2862	416	0.019
Total		14887780	1149325	100.000