

Sample Name :Amylin, amide, rat
 Lot No. :RP11280
 Cat No. :PE8431902
 Time Processed : 1:29:08
 Month-Day-Year Processed :
 03/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

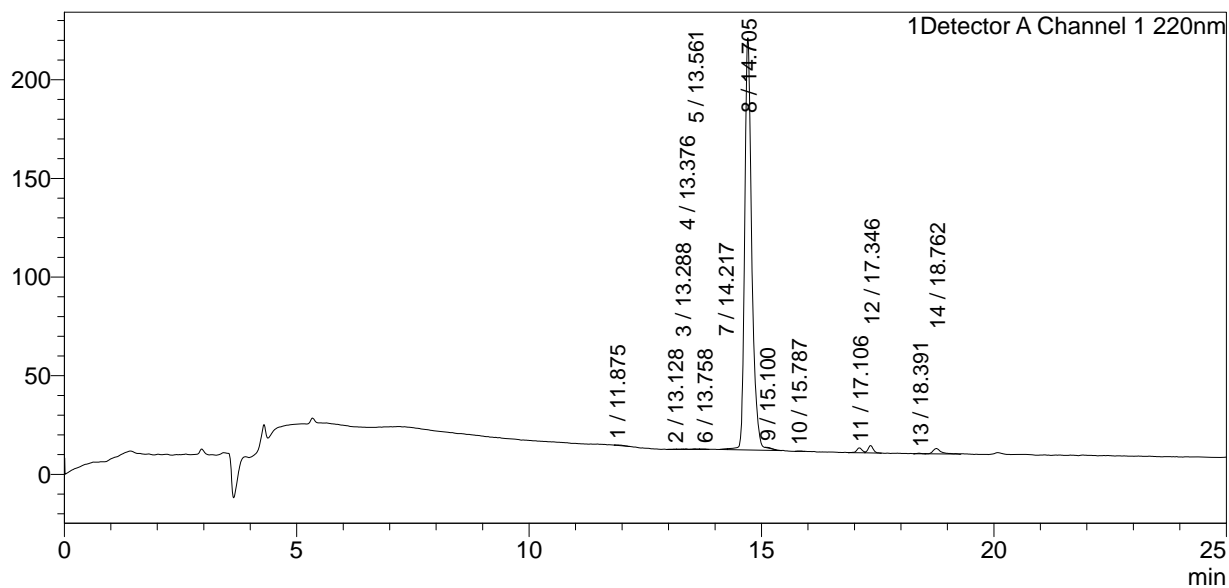

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.875	2702	141	0.117
2	13.128	1131	189	0.049
3	13.288	1562	206	0.068
4	13.376	1373	294	0.059
5	13.561	2952	344	0.128
6	13.758	2215	238	0.096
7	14.217	2443	344	0.106
8	14.705	2209838	208868	95.574
9	15.100	2105	153	0.091
10	15.787	1649	222	0.071
11	17.106	20142	2489	0.871
12	17.346	28830	3725	1.247
13	18.391	1987	302	0.086
14	18.762	33240	2714	1.438
Total		2312166	220230	100.000