

Sample Name :Uty HY Peptide (246-254)
 Cat. No. : RP20261
 Lot. No. : E7723020A
 Time Processed :7:46:51
 Month-Day-Year Processed :01/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

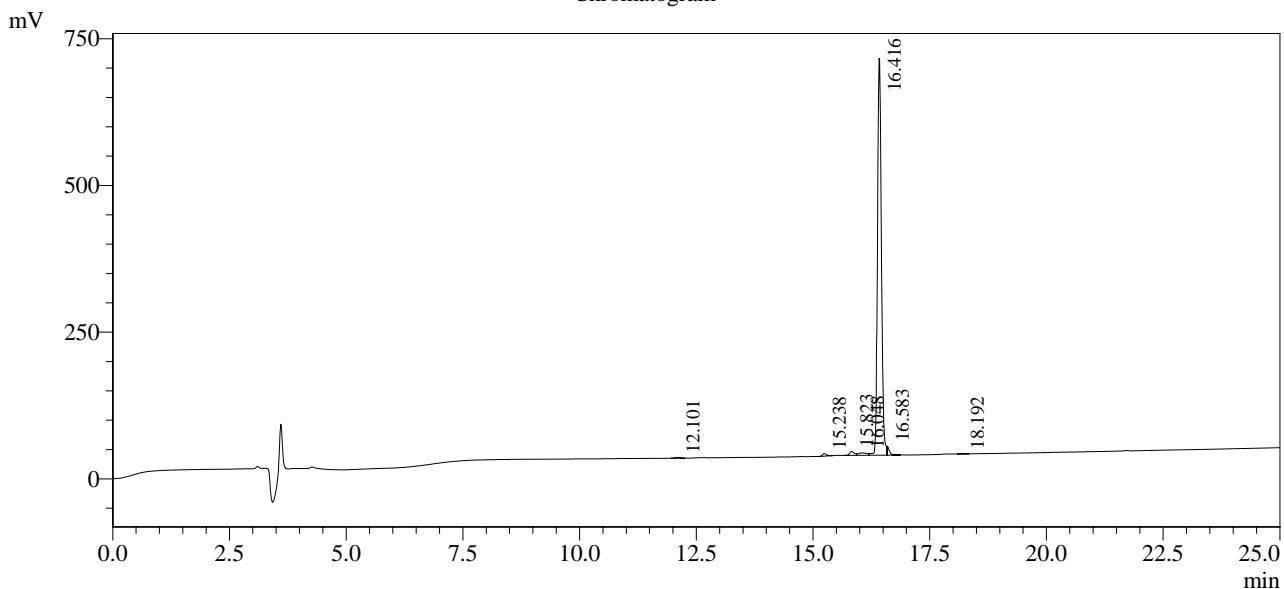

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.101	6153	1144	0.149
2	15.238	25350	4274	0.613
3	15.823	47334	6771	1.144
4	16.048	55166	4166	1.333
5	16.416	3951713	676482	95.507
6	16.583	49451	15398	1.195
7	18.192	2451	429	0.059
Total		4137618	708664	100.000