

Sample Name:[Met5]-Enkephalin
Cat No. :RP10886
Lot No. :E8884821F
Time Processed : 9:09:57
Month-Day-Year Processed : 06/17/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
10.00	Pumps	Pump B Conc.	35
35.00	Pumps	Pump B Conc.	95
37.00	Pumps	Pump B Conc.	95
37.01	Pumps	Pump B Conc.	5
42.00	Pumps	Pump B Conc.	5
42.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

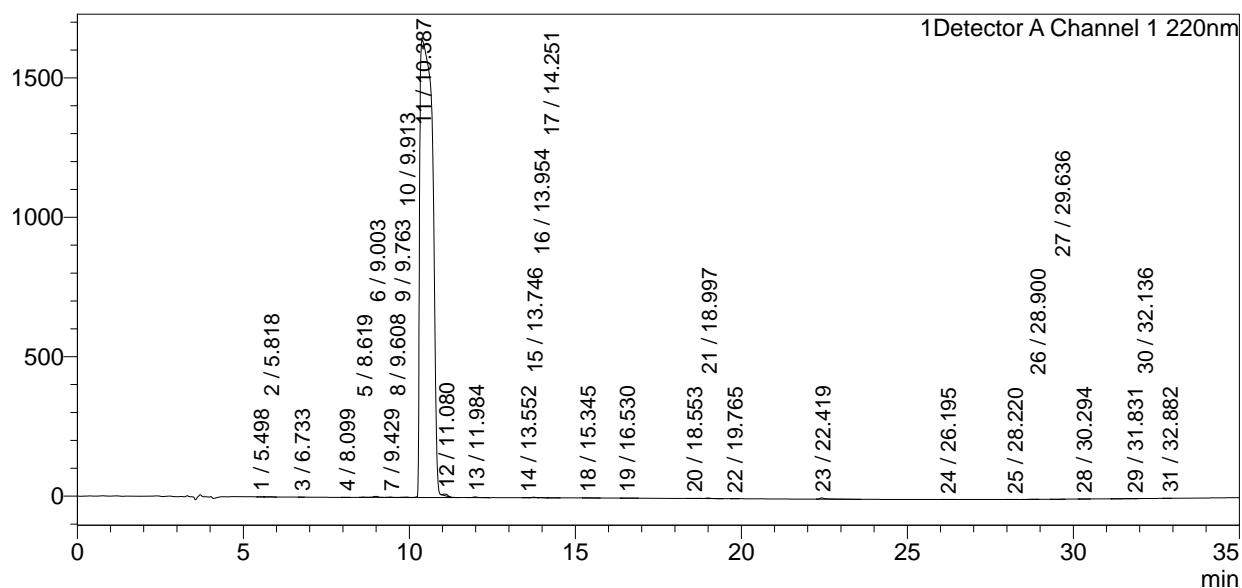

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.498	1177	191	0.003
2	5.818	7176	844	0.016
3	6.733	1678	363	0.004
4	8.099	1749	250	0.004
5	8.619	9722	1391	0.022
6	9.003	44317	3819	0.102
7	9.429	12766	1606	0.029
8	9.608	2470	427	0.006
9	9.763	5104	811	0.012
10	9.913	12427	1575	0.029
11	10.387	43201242	1641280	99.193
12	11.080	55109	5768	0.127
13	11.984	24522	2424	0.056
14	13.552	1531	216	0.004
15	13.746	16193	1860	0.037

Peak#	Ret. Time	Area	Height	Area%
16	13.954	6317	830	0.015
17	14.251	2002	200	0.005
18	15.345	12432	1024	0.029
19	16.530	3431	259	0.008
20	18.553	14669	686	0.034
21	18.997	19354	2233	0.044
22	19.765	1258	200	0.003
23	22.419	69873	4569	0.160
24	26.195	3520	459	0.008
25	28.220	1088	88	0.002
26	28.900	1167	33	0.003
27	29.636	1288	97	0.003
28	30.294	8423	1000	0.019
29	31.831	5840	262	0.013
30	32.136	3050	185	0.007
31	32.882	1709	140	0.004
Total		43552600	1675093	100.000