

Sample Name :Neurotensin
 Cat No. : RP10439
 Lot No. : E0978821C
 Time Processed :9:27:21
 Month-Day-Year Processed :03/17/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

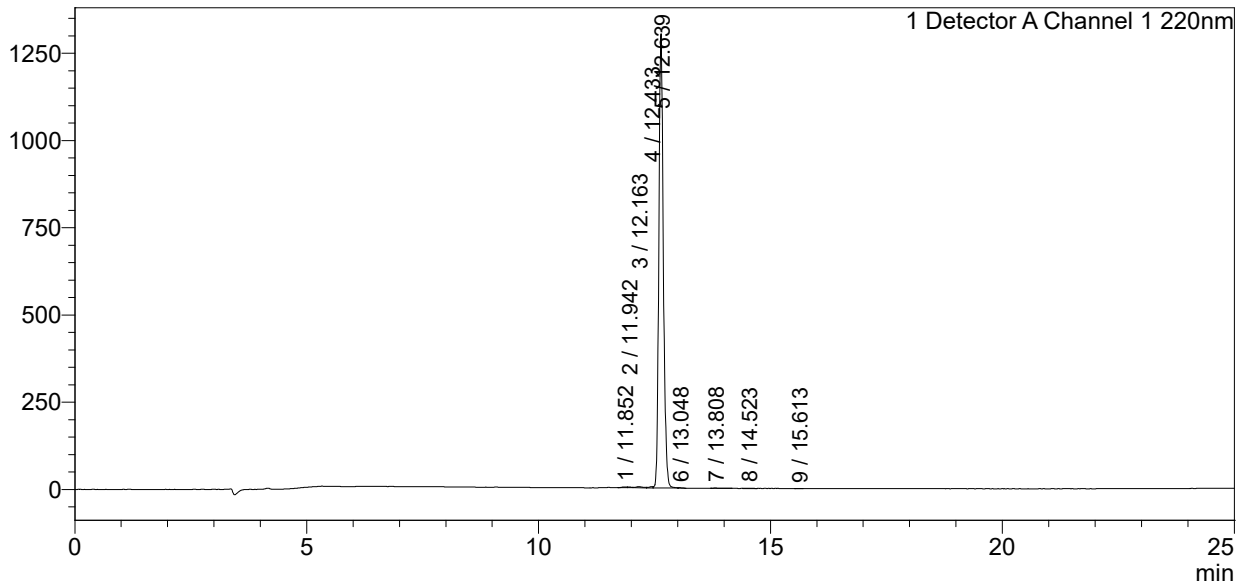

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.852	17485	2047	0.197
2	11.942	12528	2057	0.141
3	12.163	35882	3303	0.404
4	12.433	17962	3160	0.202
5	12.639	8785888	1302195	98.892
6	13.048	2501	559	0.028
7	13.808	8090	837	0.091
8	14.523	2870	239	0.032
9	15.613	1128	215	0.013
Total		8884334	1314612	100.000