

Sample Name :VIP, human, ovine, porcine, rat  
 Cat No. :RP10085  
 Lot No. :E4689819I  
 Time Processed :13:50:39  
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command         | Value |
|-------|------------|-----------------|-------|
| 0.01  | Pumps      | Solvent B Conc. | 5     |
| 25.00 | Pumps      | Solvent B Conc. | 65    |
| 25.01 | Pumps      | Solvent B Conc. | 95    |
| 27.00 | Pumps      | Solvent B Conc. | 95    |
| 27.01 | Pumps      | Solvent B Conc. | 5     |
| 33.00 | Pumps      | Solvent B Conc. | 5     |
| 33.01 | Controller | Stop            |       |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

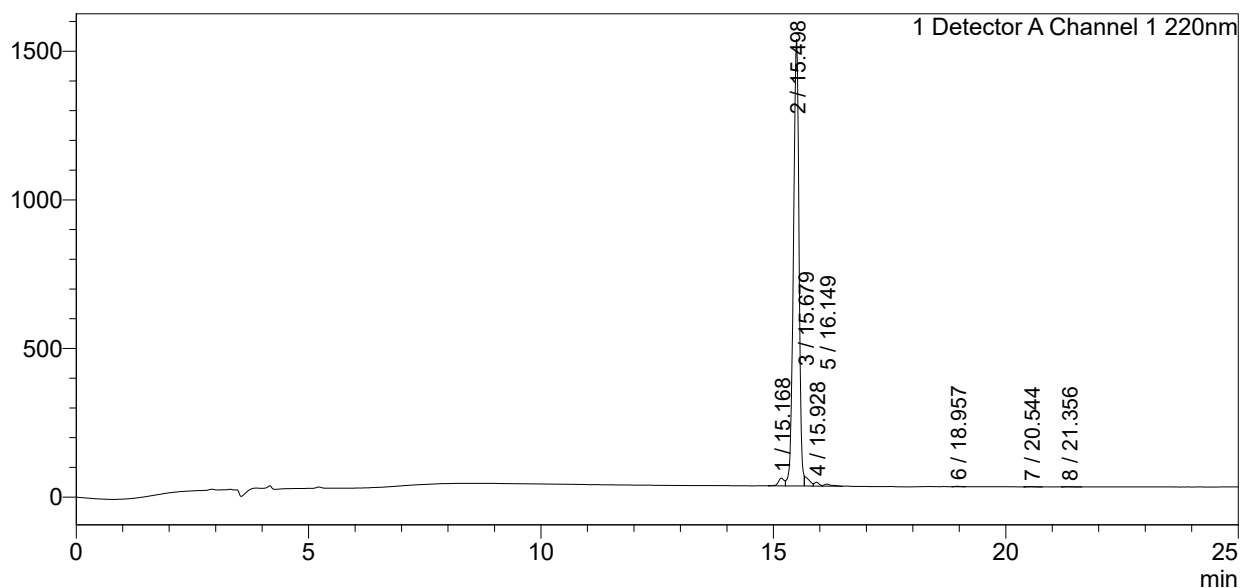

### <Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area     | Height  | Area%   |
|-------|-----------|----------|---------|---------|
| 1     | 15.168    | 226818   | 25908   | 1.727   |
| 2     | 15.498    | 12483825 | 1502202 | 95.045  |
| 3     | 15.679    | 225434   | 32073   | 1.716   |
| 4     | 15.928    | 94046    | 12948   | 0.716   |
| 5     | 16.149    | 79618    | 7315    | 0.606   |
| 6     | 18.957    | 10011    | 1422    | 0.076   |
| 7     | 20.544    | 7307     | 897     | 0.056   |
| 8     | 21.356    | 7565     | 818     | 0.058   |
| Total |           | 13134625 | 1583583 | 100.000 |