

Sample Name :Astressin
 Cat. No. : RP10980
 Lot. No. : E5463720C
 Time Processed :6:58:13
 Month-Day-Year Processed : 04/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

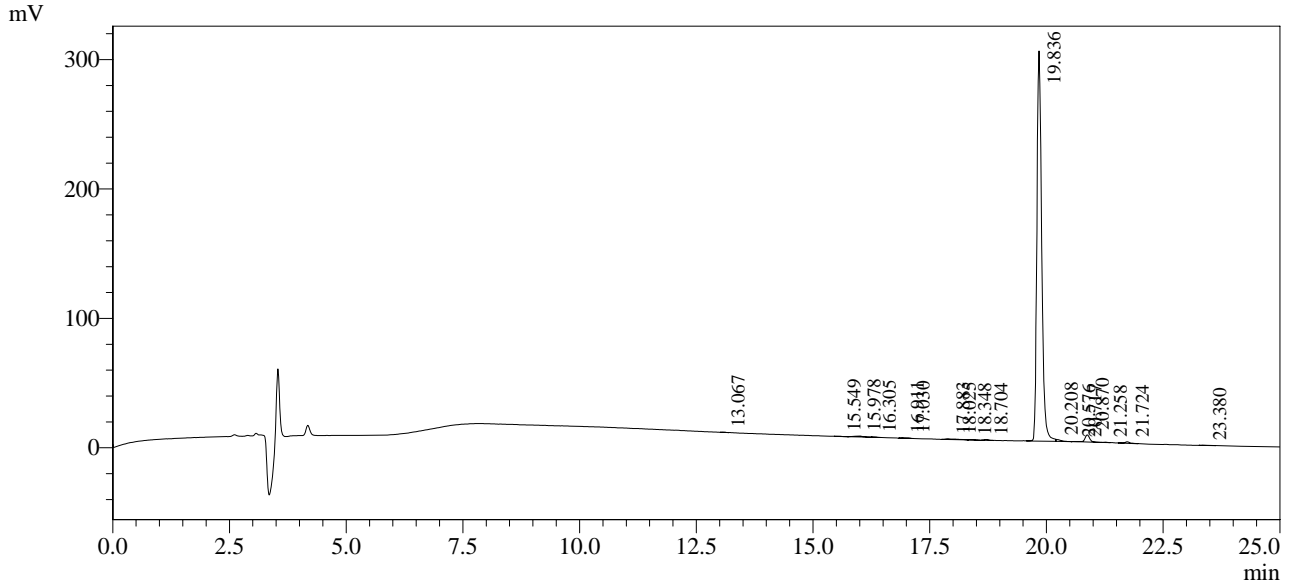

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.067	1430	258	0.063
2	15.549	1194	145	0.053
3	15.978	8548	747	0.378
4	16.305	1530	251	0.068
5	16.911	2011	324	0.089
6	17.030	1810	361	0.080
7	17.883	4762	593	0.210
8	18.025	4668	418	0.206
9	18.348	1448	99	0.064
10	18.704	3868	631	0.171
11	19.836	2167144	301583	95.780
12	20.208	10523	1564	0.465
13	20.576	1046	170	0.046
14	20.717	1172	261	0.052
15	20.870	38019	5497	1.680
16	21.258	1381	259	0.061
17	21.724	8968	1158	0.396
18	23.380	3097	382	0.137
Total		2262620	314702	100.000