

Sample Name :Autocamtide 2-amide
 Cat No. :RP20277
 Lot No. :E4872019I
 Time Processed :7:38:15
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

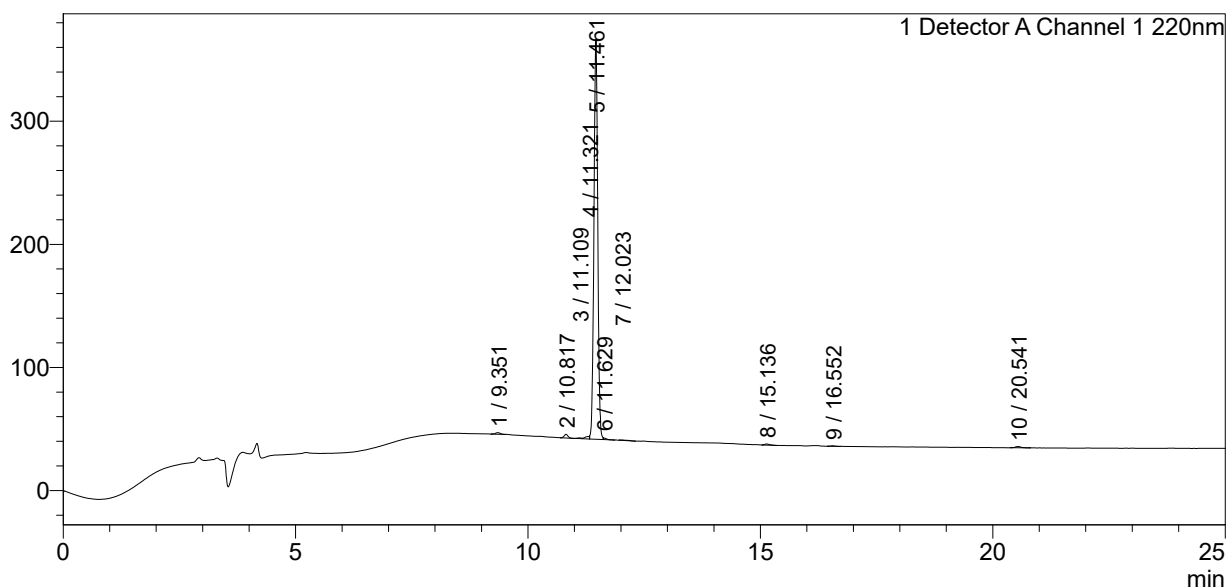

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.351	9372	1286	0.487
2	10.817	16335	2994	0.849
3	11.109	3365	578	0.175
4	11.321	12974	2134	0.675
5	11.461	1854104	324781	96.409
6	11.629	5607	1382	0.292
7	12.023	4020	375	0.209
8	15.136	6426	904	0.334
9	16.552	2039	354	0.106
10	20.541	8926	1066	0.464
Total		1923170	335854	100.000