

Sample Name : Activated Protein C (390 - 404), human
 Cat No. : RP20313
 Lot No. : E4921919I
 Time Processed : 14:51:54
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010507

<Chromatogram>

mV

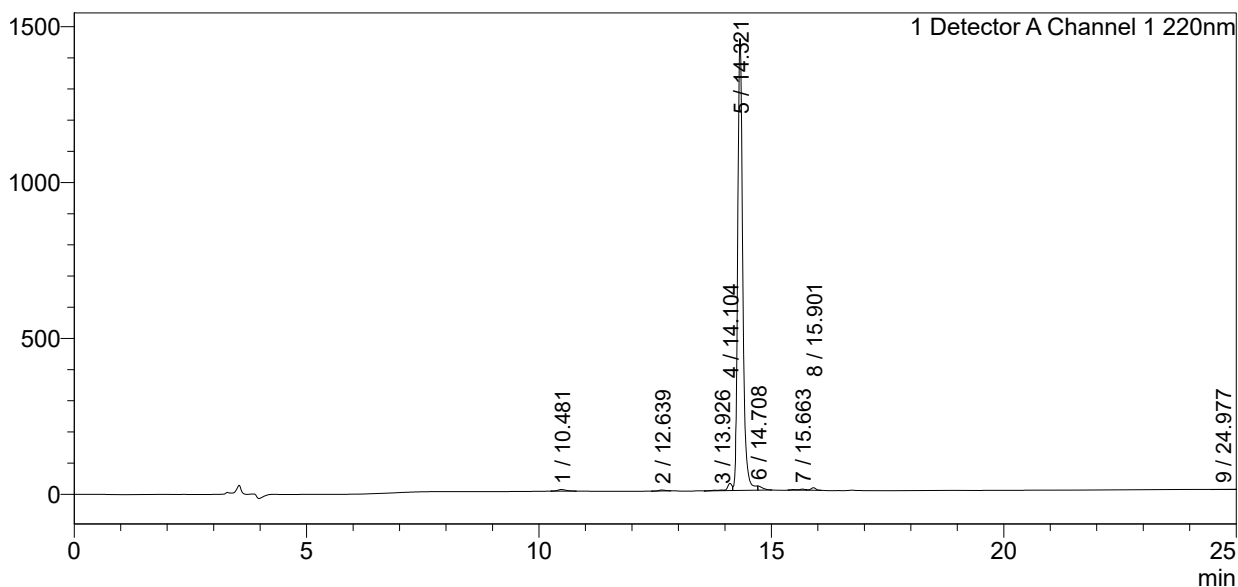

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.481	62433	5098	0.547
2	12.639	29936	3191	0.262
3	13.926	31597	2354	0.277
4	14.104	144152	23122	1.264
5	14.321	10945343	1449346	95.951
6	14.708	89947	13514	0.789
7	15.663	42095	3481	0.369
8	15.901	60224	8181	0.528
9	24.977	1469	67	0.013
Total		11407197	1508353	100.000