

Sample Name :Flu-M1 (58-66)
 Cat. No. : RP19978
 Lot. No. : PE4491710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

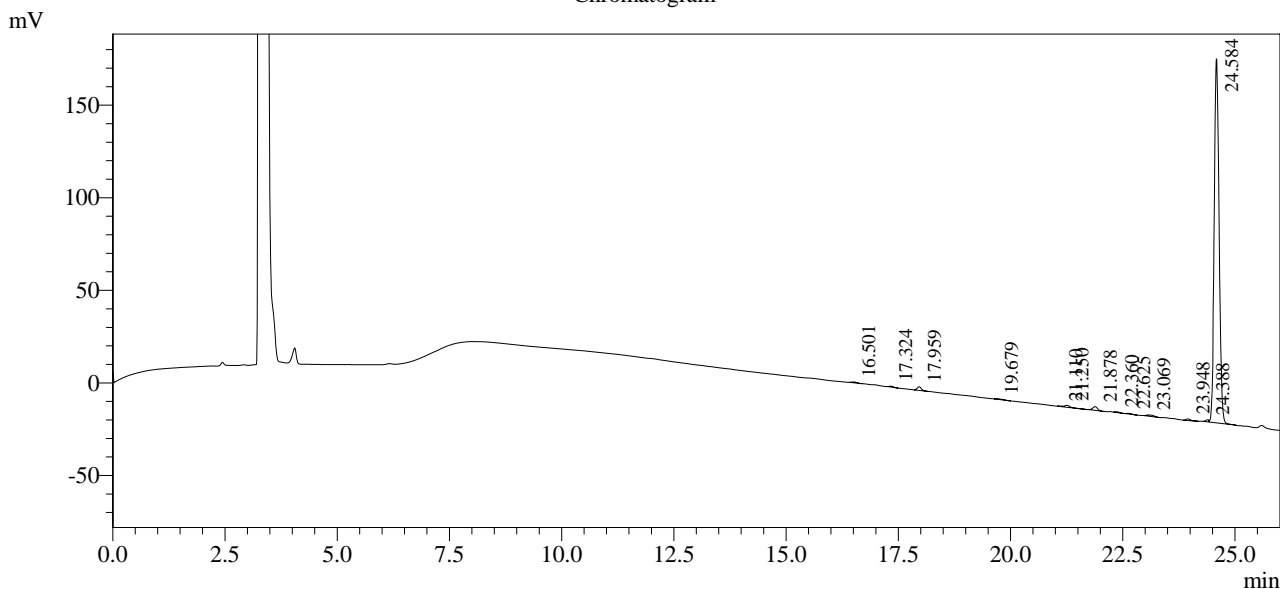

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.501	3529	425	0.226
2	17.324	3010	468	0.193
3	17.959	12004	1892	0.770
4	19.679	3262	174	0.209
5	21.110	1465	253	0.094
6	21.250	7946	1012	0.510
7	21.878	14606	2004	0.937
8	22.360	2311	359	0.148
9	22.625	2555	339	0.164
10	23.069	7691	637	0.494
11	23.948	6163	881	0.396
12	24.388	5478	1099	0.352
13	24.584	1488309	196619	95.507
Total		1558329	206162	100.000