

Sample Name :[Glu1]-Fibrinopeptide B
 Cat No. :RP20439
 Lot No. :PE2561811
 Time Processed :16:21:34
 Month-Day-Year Processed :10/31/18

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
30.00	Pumps	Pump A B.Conc	95
30.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

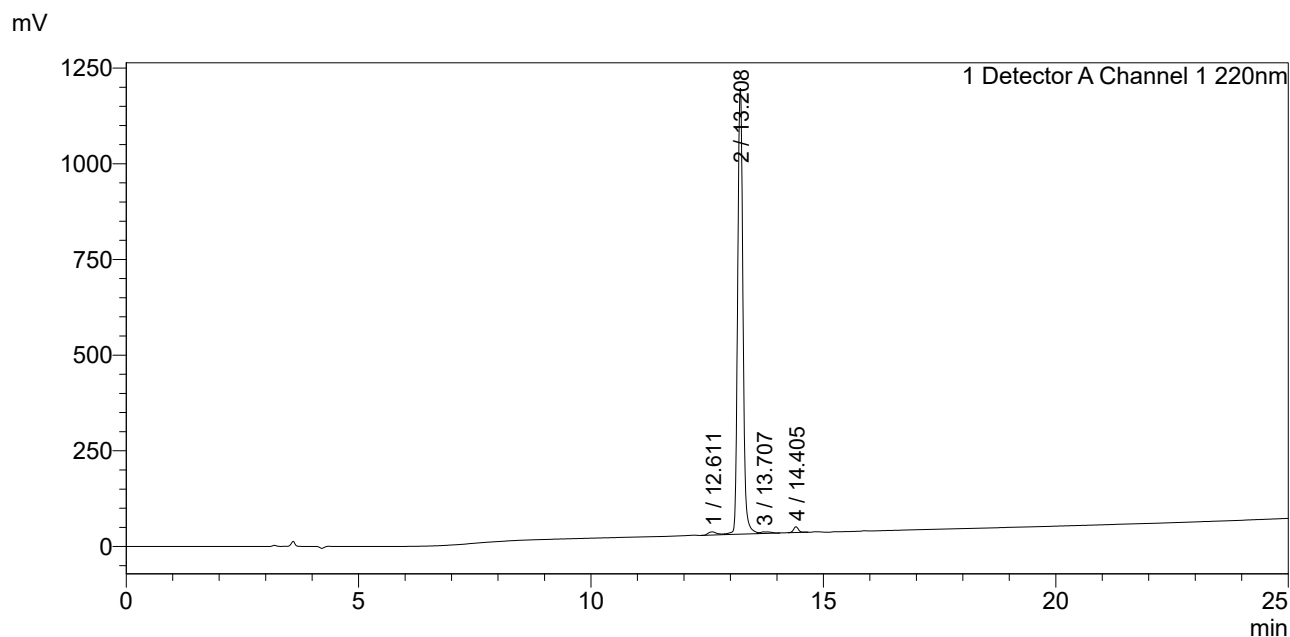

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.611	112583	8178	1.186
2	13.208	9208061	1164632	96.992
3	13.707	65410	4136	0.689
4	14.405	107600	14929	1.133
Total		9493653	1191875	100.000