

Sample Name :Substance P
 Cat. No. : RP10178
 Lot. No. : E0334819F
 Time Processed : 4:25:00
 Month-Day-Year Processed : 06/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

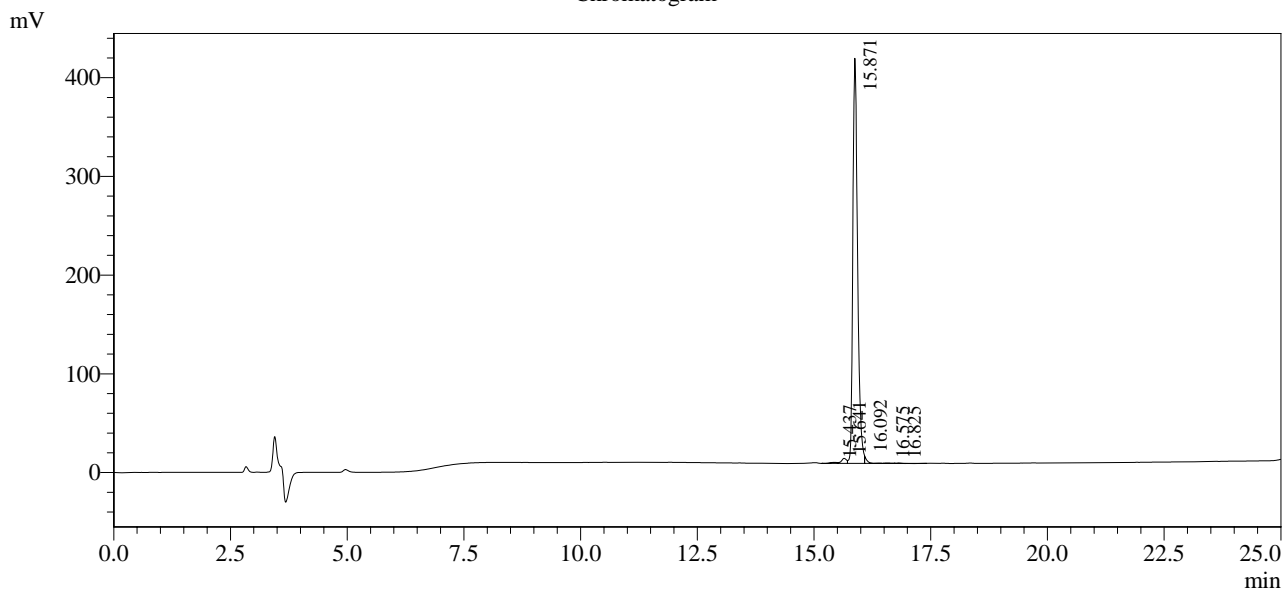

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.437	11105	1097	0.372
2	15.641	38335	5131	1.284
3	15.871	2911756	410469	97.538
4	16.092	20510	6713	0.687
5	16.575	1237	173	0.041
6	16.825	2305	378	0.077
Total		2985247	423960	100.000