

Sample Name :C3a (70-77)
 Cat No. :RP20511
 Lot No. :E4942019I
 Time Processed :10:20:33
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

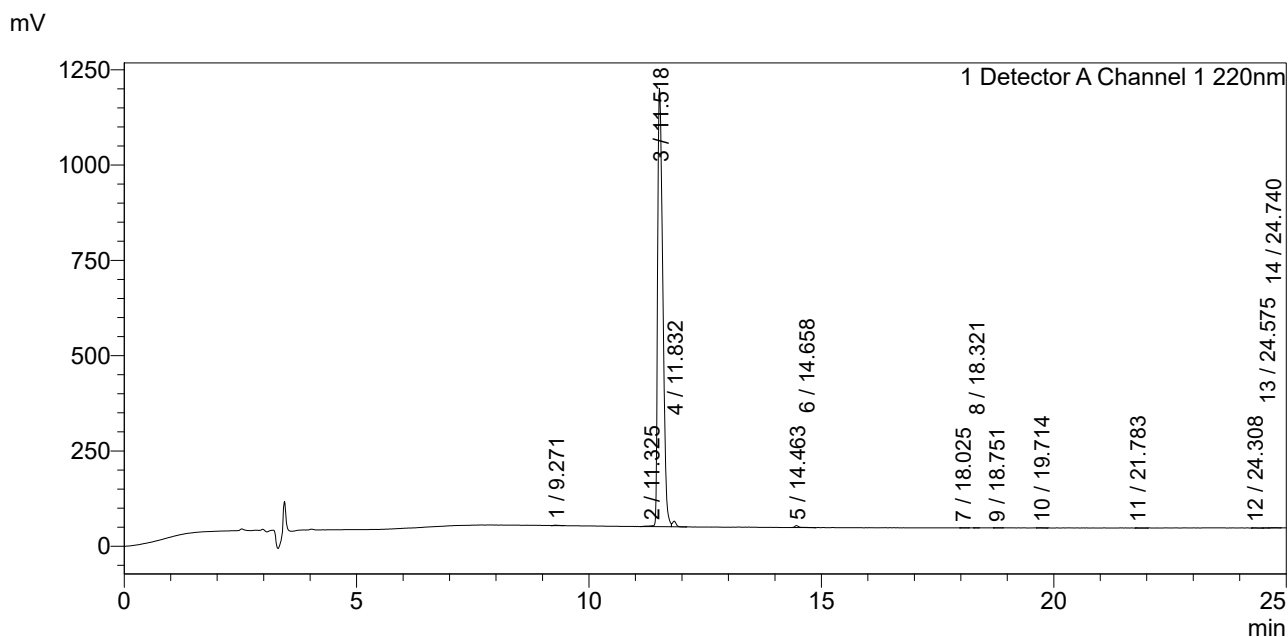

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.271	7739	990	0.085
2	11.325	16476	1962	0.182
3	11.518	8904430	1149301	98.268
4	11.832	82332	15025	0.909
5	14.463	28072	4782	0.310
6	14.658	3485	517	0.038
7	18.025	1173	173	0.013
8	18.321	1051	278	0.012
9	18.751	2300	282	0.025
10	19.714	4215	673	0.047
11	21.783	1126	202	0.012
12	24.308	1354	226	0.015
13	24.575	1467	281	0.016
14	24.740	6177	740	0.068
Total		9061397	1175434	100.000