

Sample Name : Rabies Virus Glycoprotein
 Cat No.: RP20464
 Lot No.: E9961020F
 Time Processed : 13:05:46
 Month-Day-Year Processed : 06/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

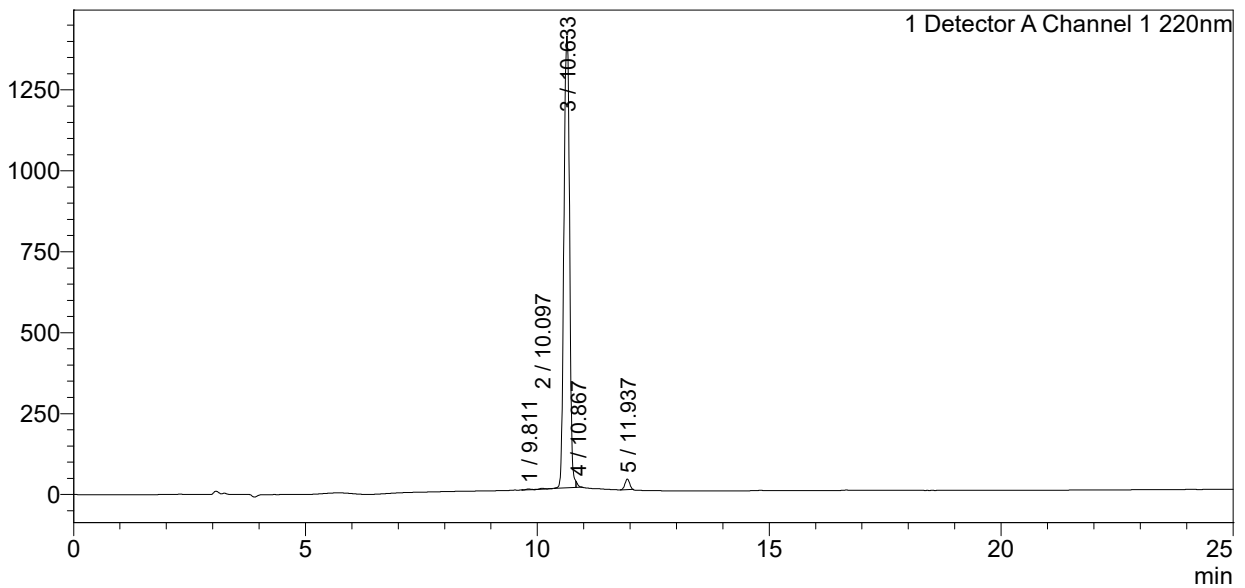

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.811	16143	2303	0.133
2	10.097	17444	2309	0.144
3	10.633	11815074	1341803	97.537
4	10.867	42907	13611	0.354
5	11.937	221831	30410	1.831
Total		12113400	1390435	100.000