


Mass Spectrum

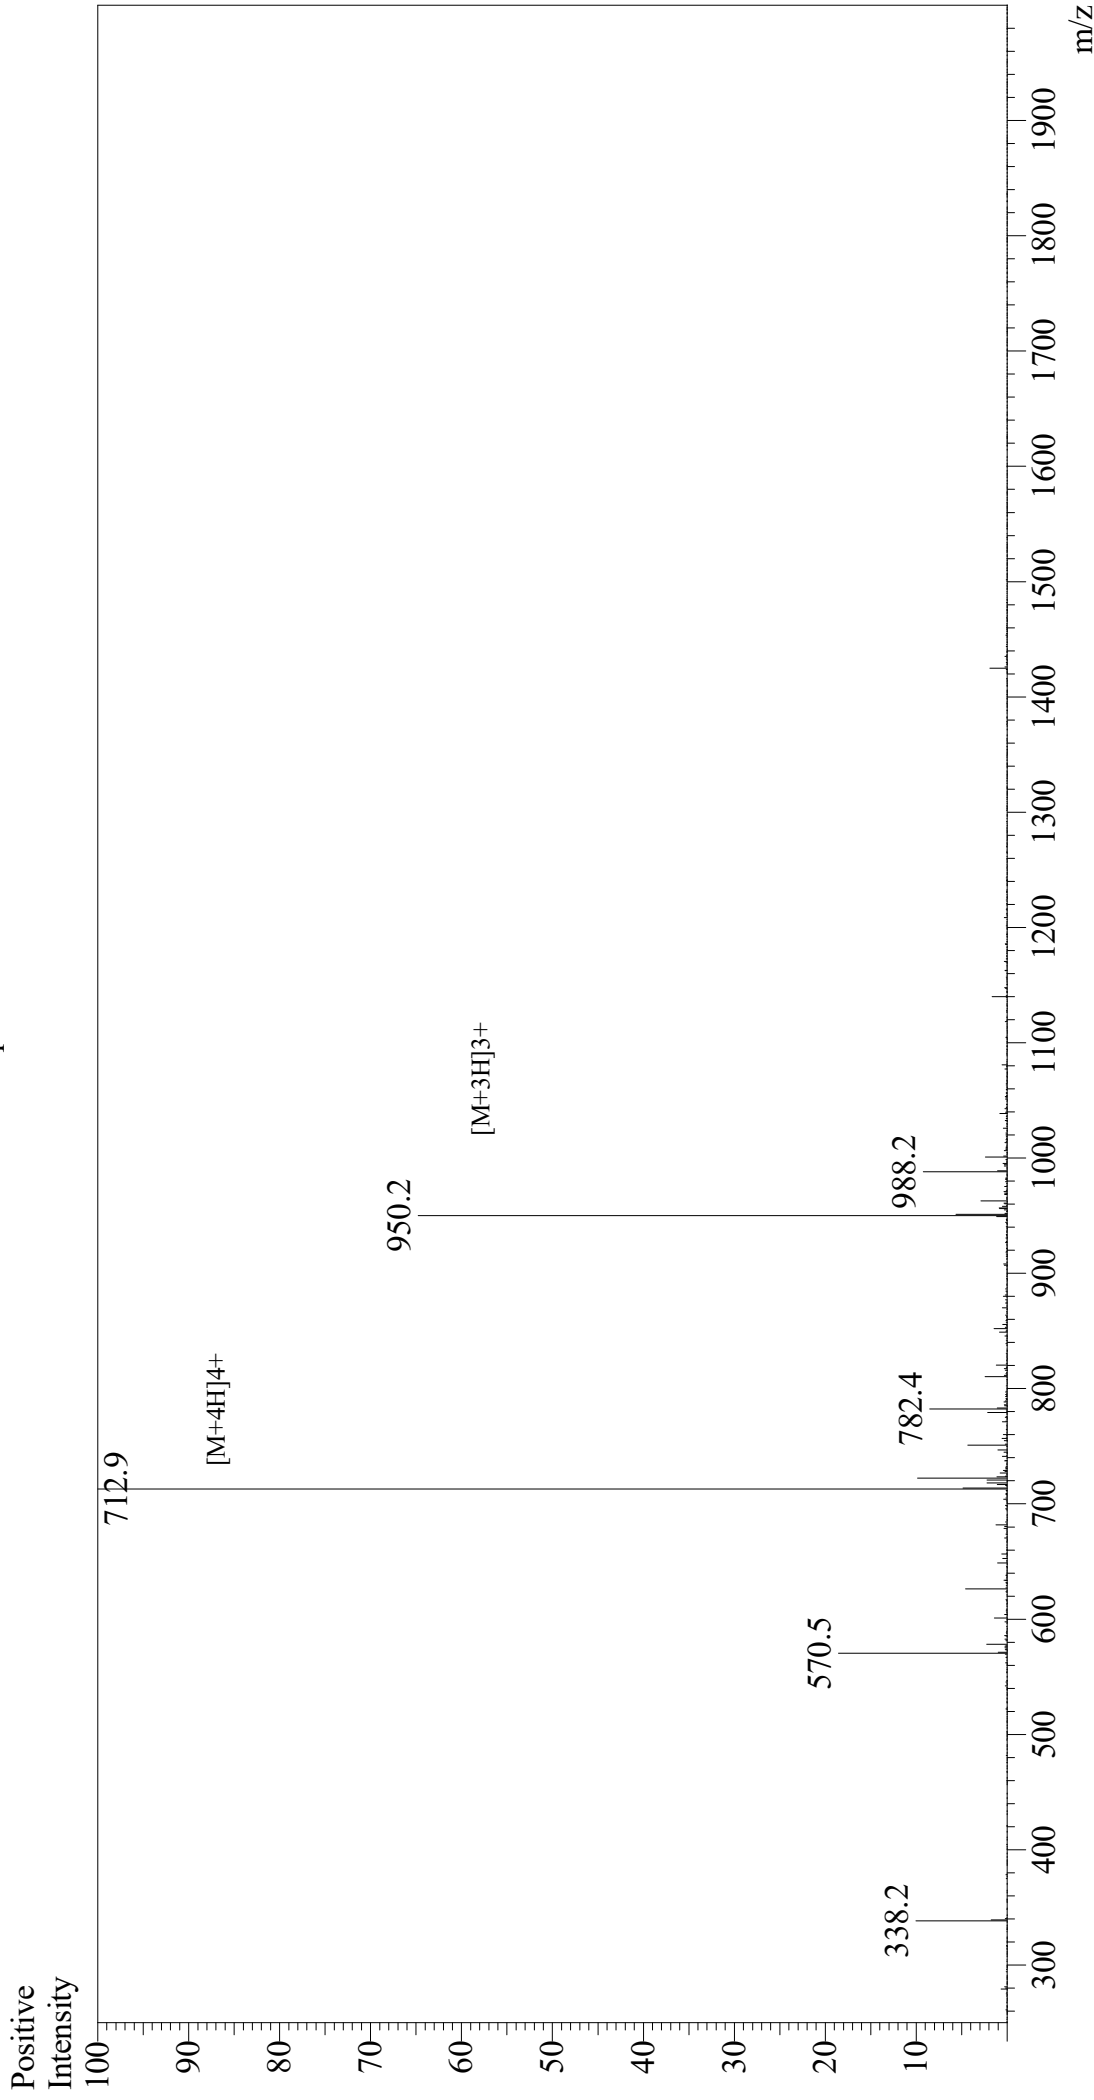

Sample Information

Month-Day Processed : 03/11/21
Time Processed : 9:09:25 AM
Injection Volume : 0.4
Sample Name : Melittin,honey bee
Cat No. : RP20415
Lot No. : E8080621C
Theoretical MW : 2847.50
Observed MW : 2847.6

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH