

Sample Name :HA Peptide
 Cat. No. : RP11735
 Lot. No. : E8605120A
 Time Processed :6:57:05
 Month-Day-Year Processed : 01/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

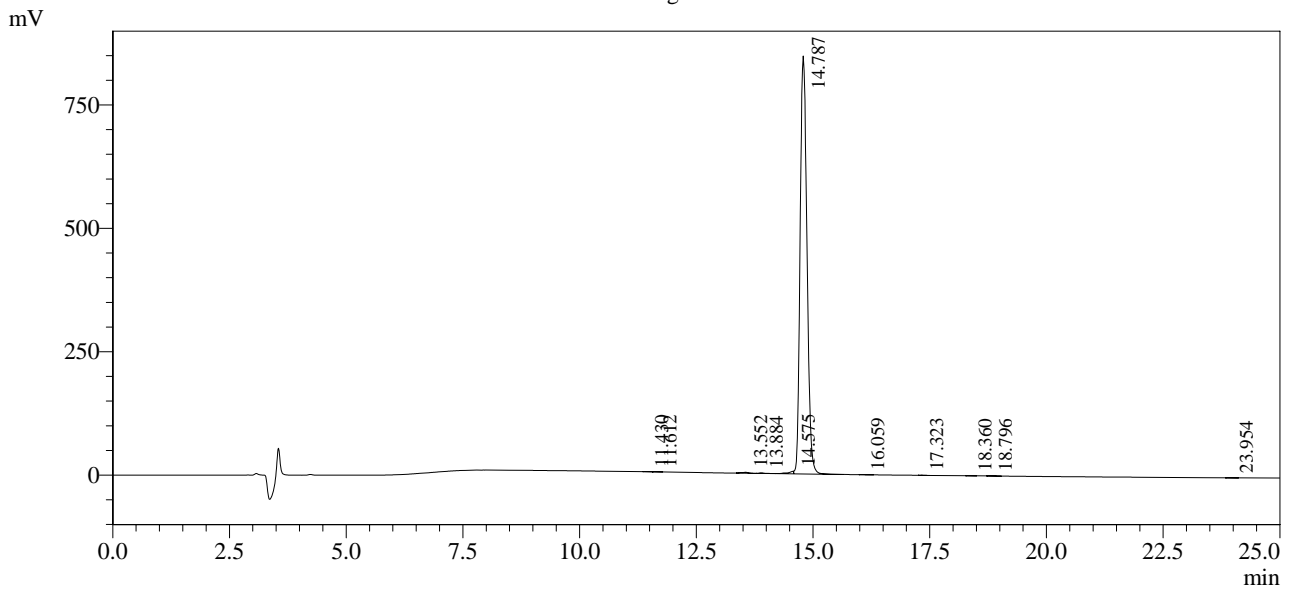

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.430	1122	178	0.013
2	11.612	1345	226	0.015
3	13.552	20763	1956	0.238
4	13.884	9051	1272	0.104
5	14.575	41021	5309	0.470
6	14.787	8635138	846957	99.034
7	16.059	1402	149	0.016
8	17.323	1729	242	0.020
9	18.360	2215	364	0.025
10	18.796	3295	474	0.038
11	23.954	2268	286	0.026
Total		8719350	857412	100.000